

# Post-Bisulfite Adapter Ligation (PBAL) Library Construction for single cells

Martin Hirst (✉ [mhirst@bcgsc.ca](mailto:mhirst@bcgsc.ca))

UBC Epigenomics Group

Tony Hui

UBC Epigenomics Group

Qi Cao

UBC Epigenomics Group

Michelle Moksa

UBC Epigenomics Group

---

## Method Article

**Keywords:** [Edit](#)

**Posted Date:** June 12th, 2018

**DOI:** <https://doi.org/10.1038/protex.2018.068>

**License:**  This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

---

## **Abstract**

This is a protocol for creating Post-Bisulfite Adapter Ligation \ (PBAL) libraries from single cells to assess the state of DNA methylation genome-wide at a single base-pair resolution.

## **Reagents**

Name	Supplier	Model or Catalogue #
Ultrapure DNase/RNase-Free Distilled Water	Thermo Fisher Scientific	10977-015
Qiagen Elution Buffer	Qiagen	19086
1M KCl	Sigma	60142-500ML-F
1M Tris-HCl –pH 8	Invitrogen	15568-025
1 M Tris-HCl –pH 7.5	Invitrogen	15567-027
Triton X-100	Sigma	X100-500ML
SDS	Sigma	L3771-500G
Protease K	QIAGEN	19131
100% Ethanol	Commercial Alcohols	
DNase I with 10X buffer	Thermo Fisher Scientific	AM2222
MethylEdge Kit	Promega	N1301
MagSi-DNA all-round Magnetic silica beads \ (20mg/mL)	MagnaMedics	MD01018
Custom Random Hexamers	IDT	Custom order
Klenow Fragment \ (3'→5' exo-) \ (50,000 units/ml)	NEB	M0212M
NEB 2 buffer	NEB	M0212M
10mM dNTP	BIOLINE	BIO-39049
Phage T7 DNA \ (full methylation of the genome prepared in house)	GeneON	310-005
Unmethylated Lambda DNA	Promega	D152A
DNA Library Prep Reagent Kit	NEB	E6000B-10
Phusion U Hot Start DNA Polymerase	Thermo Fisher Scientific	F555L
Illumina PET small forked adapter	IDT	Prepared in house
PCR primer 1.0	IDT	Diluted to 25uM
PCR primer 2.0 indexing primers	IDT	Diluted to 12.5uM

qPCR primer - human specific	IDT	Customized
qPCR primer - mouse specific	IDT	Customized
KAPA Library Quantification kit -Illumina \includes qPCR primers for library quant)	KAPA Biosystems	KK4824
SeraMag SpeedBeads Carboxylate-modified	Made in house	or Ampure XP beads
3M Sodium Acetate pH 5.5	Ambion	AM9740
Mussel Glycogen	Sigma	G1767
High Sensitivity DNA kit	Agilent	5067-4626
Qubit dsDNA HS Assay Kit	Thermo Fisher Scientific	Q32851
Qubit Fluorometer	Thermo Fisher Scientific	Qubit 2.0
AB 1400 96 Well plate \reservoir only)	Thermo Fisher Scientific	AB-1400-L
Eppendorf PCR 96-LoBind \for DNA)	Eppendorf	0030129504
Lab Marker, Fine, Black	VWR	52877-310
DNA LoBind 2.0mL tubes	Eppendorf	022431048
Qubit Assay tubes	Thermo Fisher Scientific	Q32856
Gilson P2 pipetman	Mandel	F144801
Gilson P10 pipetman	Mandel	F144802
Gilson P20 pipetman	Mandel	F123600
Gilson P100 pipetman	Mandel	F123615
Gilson P200 pipetman	Mandel	F123601
Gilson P1000 pipetman	Mandel	F123603
<b>Thermo Mixer</b>	Eppendorf	5382000023
<b>Multi 12-channel Pipette P20</b>	Rainin	17013803
<b>Multi 12-channel Pipette P200</b>	Rainin	17013805
<b>Clear Plastic Plate Cover \not for PCR)</b>	Edge Bio	48461
<b>PCR cover</b>	Bio Rad	MSD-1001
<b>Microseal 'F' foil Seals \metal covers)</b>	Bio Rad	MSF 1001

Eppendorf 5810R centrifuge \(tube)	Eppendorf	
Eppendorf 5424R centrifuge \(plate)	Eppendorf	
ViiA 7 Real-Time PCR System	Applied Biosystems	
MicroAmp Optical 384-well reaction plate	Applied Biosystems	4309849
MicroAmp Optical Adhesive film	Applied Biosystems	4311971
Agilent 2100 Bioanalyzer	Agilent	G2939BA
SafeTouch Advanced Stretchy gloves	Medicom	1137 A, B,C,D
MAGNUM FLX magnet	Alpaqua	A000400
Vortex	Mandel	S0100A
Table Minifuge	Mandel	C1801
1.2 mL Storage Plate	Thermo Fisher Scientific	AB-1127
Axygen 96 square deep-well	Axygen	P2MLSQCS
Axygen Assay Plate	Axygen	P96450VCS
P10 Pipette tips	Gilson	DFL10ST
P100 Pipette tips	Gilson	DFL100ST
P200 Pipette tips	Gilson	DFL200ST
P20 Pipette tips	Gilson	DFL20ST
P1000 Pipette tips	Gilson	DFL1000ST
Biological Safety Cabinet \(housing for Bravo)	Baker	Class II Type A2
Laminar flow hood \(PCR workstation)	Erlab	Biocap 391
Bravo Automated Liquid Handling Platform	Agilent	Bravo
UV crosslinker	Analytik Jena	CL-1000
RNase Away \(4X4L)	Fisher Scientific	14-754-34
DNA Away \(250mL)	ThermoFisher	7010PK
CoolRack XT PCR96 \(for plates)	BioCision	BCS-529
TruCool® Midi 4L Ice Pan	BiCision	BCS-113
50mL Falcon tubes	Fisher Scientific	1443222

CoolRack® M15 \for tubes/enzymes)	BiCision	BCS-125
DNA LoBind tube 1.5mL	Eppendorf	022431021
DNA LoBind tube 0.5mL	Eppendorf	022431005
MicroAmp™ Adhesive Film Applicator	ThermoFisher	4333183
CoolRack XT PCR384	BiCision	BCS-538

## 1. Oligos

### 2. qPCR primer for human \(HG19)

Forward: 5'-TGTTTGTAAAGTTATAAGTGGATA-3'

Reverse: 5'-CAAAAAAAATTACTAAAAATTCTTCT-3'

### 2. qPCR primer for mouse \(mm10)

Forward: 5'-AAAATTGAAAATTATGGAAAATGAG-3'

Reverse: 5'-CCAAATCCTTCAATATACATTCTC-3'

### 3. qPCR primers for library quantification \(supplied in the Kapa Lib Quantification Kit - Illumina)

Forward \(P1): 5'-AAT GAT ACG GCG AC ACC GA-3'

Reverse \(P2): 5'- CAA GCA GAA GAC GGC ATA CGA-3'

### 4. Illumina PET small forked adapter oligos \(PAGE purified and hybridized together):

DNA Oligo 1: 5'- /5Phos/GAT CGG AAG AGC GGT TCA GCA GGA ATG CCG AG -3'

*Note: 5' Modification: Phosphorylation*

DNA Oligo 2: 5' - ACA CTC TTT CCC TAC ACG ACG CTC TTC CGA TC\*\*T - 3'

*Note: 3' Modification: \*\*T is a phosphorothioate bond*

### 5. PCR Primers \(GSC construct):

Primer 1.0: 5'-AAT GAT ACG GCG ACC ACC GAG ATC TAC ACT CTT TCC CTA CAC GAC GCT CTT CCG ATC T -3'

Indexing primers 2.0 \(GSC construct): 5'-CAA GCA GAA GAC GGC ATA CGA GAT NNNNNN CGG TCT CGG CAT TCC TGC TGA ACC GCT CTT CCG ATC T-3'

## 6. Custom Random Hexamers

5'- NNNN\*\*N\*\*N-3' *Note: Modification: \* = phosphorothioate bond*

# Procedure

## 1. Procedure

## 2. General Guidelines

- 1. Read this entire document and *EGL005.03 96 well Library Construction using Agilent Bravo* SOP before starting this procedure for the first time.
- 2. Given the nature of single cell work, it is crucial to always wear gloves when handling sample plates, reagents and equipment, and to treat everything with clean PCR techniques. Use two layers of gloves and switch the outer gloves anytime something outside of the dedicated single-cell laminar flow hood is handled. Use a disposable lab coat throughout this procedure.
- 3. All work should be performed inside a dedicated single-cell work only enclosed PCR workstation and an enclosed Bravo liquid handler.
- 4. Before starting, turn on the PCR workstation, place a clean autoclave bag in the waste container, clean all work surfaces and equipment such as pipettes, centrifuge, vortex thoroughly with RNase Away or DNA Away spray.
- 5. Use Eppendorf LoBind PCR clean plates for samples and the less expensive AB-1400-L plates as reservoirs.
- 6. Seal all plates with a plastic EdgeBio cover every time they exit the hood and never re-use covers. Use MicroAmp adhesive film applicator to create a good seal around each well.

- 7. Keep the samples and brews on ice. Enzymes should only be taken out of the freezer just before addition to the brew, transported only in a designated pre-chilled to -20°C cold-block \ (CoolRack M15), then immediately returned to the freezer.
- 8. Plates should never be vortexed. Plate mixing steps are only to be done using 12-channel pipette or using the Bravo.
- 9. When placing plates on the Bravo deck, make sure that the A1 well is always in the upper left corner.
- 10. All reagents except enzymes should be aliquoted for single use. All buffers should be well mixed by repeated pulse-vortexing before addition to the brew. All brews should be well mixed by repeated *gentle* pulse-vortexing before dispensing into reservoir to assure an equal distribution of all components and thus uniformity of enzymatic treatments across a plate.
- 11. At the end of each working day, discard all used plastic ware and remove the waste bag first, then wipe down all work surfaces with RNase Away or DNA Away.

## 2. Reagents to prepare in advance

- 1. Spike-In mix preparation:
- 1.1. In a LoBind 1.5mL PCR clean Eppendorf tube, prepare equal mass mix of: methylated T7 gDNA and unmethylated lambda gDNA and dilute to 20ng/uL with Qiagen EB buffer. Aliquot for single use and store at -20°C. Prepare 1ng/uL dilution of the mix using Qiagen EB buffer, check the quant using Qubit HS Assay, aliquot for single use, and store at -20°C for up to 3 months.

- 1.2. Retrieve one aliquot of 1ng/uL Spike-In mix and dilute to 6pg/uL using Qiagen EB buffer, mix very well by repeated pulse-vortexing, and aliquot single use. Store in a LoBind Eppendorf tubes at 4°C for up to two weeks \scPBAL Box).
- 2. Positive control preparation:
  - 2.1. In a LoBind 1.5mL PCR clean Eppendorf tube, prepare 2.5ng/uL dilution of HL60 gDNA using Qiagen EB buffer, mix very well by pipetting \do not vortex, and check the quant using Qubit HS Assay. Aliquot for single use \(6uL/tube) and store at -20°C for up to 6 months.

## DAY 1

### 3. Single cell Lysis

- 1. The input for this procedure is a plate containing single cells \or nuclei sorted into 384-well plate \Quadrant A only – see image below for sorting plate layout) and snap frozen dry in liquid nitrogen or ethanol/dry ice bath.

See figure in Figures section.

- 2. Prior to starting this procedure confirm the plate layout with the supervisor to determine the location of single cell and 10 cell wells within the 384 well plate.
- 3. Put a fresh pair of gloves, get fresh ice and keep the ice pan outside of the PCR workstation for now. Check -20°C freezer \20-1 to make sure that a chilled Coolrack XT PCR96 and Coolrack M13 are ready. Turn on the PCR machine and place a piece of tape on it to indicate it is in use.
- 4. Put on a new disposable lab coat, turn on the PCR work station and clean the single-cell PCR space and equipment as per instructions in General Guidelines, section 1.0 above. Wipe down the ice bucket with RNase or DNA Away before placing it inside the now clean single-cell work station.
- 5. Retrieve one aliquot of 2.5 ng/uL stock of HL60 gDNA from 4°C \scPBAL Box) and keep it on ice.

- 6. Retrieve one aliquot of 6pg/uL of Spike-In mix from the 4°C fridge and keep it on ice. Using LoBind tube \labeled as SC spike-in), make 100X dilution by mixing 2 uL of the Spike-In mix with 198 uL of Ultrapure distilled water \labeled as SC spike-in). This should yield 60fg/uL concentration. Mix very well by multiple pulse-vortexing. Keep it on ice.
- 7. Inside the PCR work station, working on ice, in a LoBind 1.5mL tube, prepare the **Lysis brew** according to the following calculator:  
[See figure in Figures section.](#)
- 8. All reagents \labeled as enzymes) must be pulse-vortexed and spun down in a minifuge before addition to the brew. Add enzyme last. Mix enzyme by gently flicking the tube then spin down in a minifuge before addition to the brew.
- 9. After addition of all of the components, pulse-vortex the brew multiple times to assure an even distribution of all components. Quick spin the brew in a minifuge and keep it on ice.
- 10. Working on ice, aliquot 40uL/well of the Lysis brew \labeled as (4uL X 8 rows + extra) into **row A** of a fresh AB 1400L 96-well reservoir plate. Seal the plate with EdgeBio cover and spin down at 3000rpm for 1min, 4°C. Keep the plate on ice. This plate will be used as a reservoir \labeled as "RV" and mark the row).
- 11. Retrieve 384-well single cell sample plate from the -80°C freezer and spin it down for 2 minutes at 3000rpm at 4°C. Place the plate on ice. Mark the rows and columns that contain samples.
- 12. Working on ice, using a P20 multichannel pipette, add 4uL/well of Lysis buffer into each sample well of the 384-well plate \labeled as (according to plate layout – quadrant A only). After each row addition, pipette up and down 10 times to mix. Try not to create bubbles. Change tips between rows. If there is a re-arrangement of well locations - note the changes in your lab book.
- 13. Seal the "**RV**" plate with a EdgeBio cover and save it for later. Seal the 384-well sample plate with EdgeBio cover and spin down at 3000 rpm, 4°C for 1min.

- 14. Working on ice, using P20 multichannel pipette set to 6 uL, transfer all 4 uL from each sample well into a new LoBind 96-well plate except M1, M3, O1, O3, label this plate “**scPBAL DNA**”. In the new LoBind 96-well plate, make sure to leave 4 wells empty for 3 negative controls \ (G2, H1 and H2) and one positive HL60 gDNA control \ (G1).
- 15. To the 3 negative control wells: G2, H1, and H2 add 4ul of Lysis buffer \ (take the buffer from the Lysis buffer reservoir plate). Leave G1 well empty.
- 16. Seal the 96-well sample plate with a **BioRad** PCR cover using MicroAmp adhesive film applicator as follows:
  - 16.1. After placing the PCR cover on, using adhesive film applicator apply firm pressure to press the cover onto the plate.
  - 16.2. Run the applicator firmly from left to right several times. Run the applicator up and down several times. Create a good seal around each well.
  - 16.3. Run the edge of the applicator around the border to seal the edge wells.
  - 16.4. Repeat the left to right and up and down motions to assure a good final seal.
  - 16.5. Inspect each well to make sure that each well edge is imprinted on the PCR cover.

*Note: Using the applicator's edge to seal between the wells is NOT recommended. It may actually pull the seal off the wells.*

- 17. Spin the plate at 3000 rpm, 4°C for 1min. Place the plate in a pre-heated to 50°C PCR machine \ (record PCR machine number) and close the lid. Use program: **sc-lysis** to incubate at 50°C for 30 minutes followed by a 4°C hold \ (with heated lid). While the plate is incubating, pre-treat the silica beads with DNase I \ (see step 4 below).
- 18. After the 30min incubation is complete, spin the plate at 3000rpm for 1min at 4°C.

- 19. Keep the “scPBAL DNA” plate on ice. If necessary, store the plate at -20°C overnight as this is a safe stopping point.

#### 4. DNase I treatment of silica beads

- 1. Retrieve an aliquot of silica beads from the 4°C fridge \ (BOX: MagSi beads). Gently pulse-vortex the tube thoroughly until the solution is uniformly dark brown and there is no longer a bead pellet on the bottom of the vial.
- 2. Calculate total amount of beads required using the calculator below. For a full plate the volume is 230 uL.

[See figure in Figures section.](#)

- 3. Aliquot the beads equal volume \ (115 uL) into 2 wells: B1 and B2 of the “RV” reservoir plate.
- 4. Place the plate on the Magnum FLX magnet \ (wipe down the magnet before placing it inside the hood) and incubate at room temperature for 2 min until the beads separate and the solution becomes clear.

[See figure in Figures section.](#)

- 5. Using P200, carefully remove the supernatant without disturbing the beads.
- 6. Take the plate off the magnet and resuspend the beads in each well with 115uL of Qiagen EB buffer. Mix up and down few times.

- 7. Place the plate back onto the magnet for 2 min until the solution becomes clear.
- 8. While the beads are on a magnet, working on ice, prepare **DNase I master mix** according to the following calculator:
- 9. All reagents \ (except enzymes) must be vortexed and spun down in a minifuge before addition to the brew.
- 10. Add all of the non-enzymatic components first and mix very well by repeated pulse-vortexing. Keep it on ice.
- 11. Enzyme should be added last. Transport the enzyme from -20°C freezer to the PCR workstation in a pre-chilled to -20°C Coolrack M13 \ (for tubes).
- 12. Mix the enzyme by flicking the tube several time, quick spin in a minifuge, and place it back in the chilled tube coolrack.
- 13. When pipetting the enzyme, aspirate slowly as the solution is viscous. After dispensing the enzyme into the brew, pipette up and down several times to rinse the tip.
- 14. Immediately return the enzyme back to the -20°C freezer before proceeding.
- 15. Mix the entire brew very well by gentle pulse-vortexing, spin down in a minifuge and keep it on ice.
- 16. With the “RV” plate still on the magnet, carefully remove the supernatant. Do not disturb the beads.
- 17. Remove the plate from the magnet and resuspend each well with beads in 115 uL of DNase I master mix. Mix each well very well by pipetting up and down 10 times.

- 18. Seal the plate very well with a BioRad PCR cover. Do not spin down.
- 19. Place the plate in a PCR machine pre-heated to 37°C and close the lid. Use program: sc-dnase1: 37°C for 30 minutes, 70°C for 10 minutes, 4°C hold.
- 20. After DNase I treatment is complete, remove the plate from the PCR machine and keep it on ice. Split the mixture equally over one full row and seal the plate with EdgeBio cover. This will be 19 uL per well. *Note: DNase I treated silica beads can be stored at 4°C overnight.*

## 5. MethylEdge bisulfite conversion

- 1. Prepare the MethylEdge Conversion mix using the following calculator:
- 2. Aliquot the Conversion Mix 310uL/well into **one** row of the “RV” plate. Mark the row.
- 3. Get the “scPBAL DNA” plate, add the 4 uL \(10ng) HL60 gDNA into the positive control well -G1.
- 4. Using P200 multichannel pipette, add 33.5uL of the Conversion **mix** prepared above into each row of the “scPBAL DNA” plate \(except negative control wells) and mix 10 times by pipetting up and down. Change tips between rows. Make sure to manually take off the tips corresponding to the 3 negative control wells: G2, H1 and H2. Make sure to add the mix to the positive control well – G1.
- 5. Using P100 single channel pipette, add **33.5uL** of MethylEdge Conversion **reagent only** \WITHOUT the spike-in controls) into the 2 negative control wells: H1 and H2 and mix 10 times by pipetting up and down.
- 6. Seal the plate with a BioRad PCR film and spin it down for 1 minute at 3000 rpm at 4°C.

- 7. Place the plate in a PCR machine, close the lid and incubate using program **bs-prg1** \ (with a heated lid):

98°C for 8 min

54°C for 60 minutes

4°C forever

- 8. While the plate is incubating, UV-treat the reagents as outlined in step 6 below.
- 9. After the incubation of bisulfite conversion completes, spin the plate at 3000g for 1min, 4°C and proceed to the Desulphonation. Keep the plate covered to minimize the exposure to light.

## 6. sc Desulphonation reagent preparation – UV treatment

- 1. Retrieve one tube of NEB 2 buffer from -20°C and place it on ice.
- 2. Prepare Binding buffer + Beads mixture:
  - 2.1. Get a new 96well plate and label it “Binding+Beads”.
  - 2.2. Mix the DNase I treated silica beads in the “RV” plate by pipetting up and down at least 10X.
  - 2.3. Using a P20 multichannel, add 2uL of the DNase I treated beads into each well of “Binding+Beads” plate. No need to change tips between rows. Cover and save the “RV” plate.
  - 2.4. Pour MethylEdge Binding buffer into a clean reservoir. Using P200 multichannel, aliquot 180uL per well into “Binding+Beads” plate. Mix the beads and binding buffer very well by pipetting up and down at least 10X until it is homogenous light brown. No need to change tips between rows. Make sure that the solution is fully homogenous before moving forward.

Cover with a plastic seal and keep it at **room temperature**.

- 2.5. Collect the leftover buffer from reservoir back to Binding Buffer bottle.
- 3. Prepare the Desulphonation plate:
  - 3.1. Get another new 96well plate and label it “Desul”.
  - 3.2. Pour around 8 mL MethylEdge Desulphonation buffer into a clean reservoir and using P200 multichannel, aliquot 65uL per well into “Desul” plate \ (equivalent to the number of reactions). Cover the plate with a plastic seal and keep it at room temperature.
- 4. Pour Qiagen EB buffer into a clean reservoir and using P200 multichannel, aliquot 30uL per well into a 96 well plate \ (equivalent to the number of reactions). Cover the plate with a plastic seal, label “EB”, and keep it at room temperature.
- 5. Using sterile 50mL falcon tubes, prepare two tubes of 50mL 80% ethanol \ (mix 40mL of 100% ethanol with 10mL of ultrapure water). Mix very well.
- 6. Use aluminum foil to cover the inside of the ice box, shiny side up and filled with ice. Put the plates, ethanol, and NEB2 buffer in the ice box. Treat all 3 plates: “Binding + Beads”, “Desul”, “EB”, the tube of NEB 2 buffer, and both 50mL falcon tubes of 80% ethanol in a UV crosslinking machine for a total of 60min. \ (UV crosslink: set to 60 minutes, located at MSL).

## 7. sc Desulphonation reaction and DNA purification

- 1. Turn on the Eppendorf thermomixer and preheat to 56°C by “spinning” at 0 rpm. Place two plate coolracks at -20°C door shelf to chill.
- 2. Turn on the Agilent computer and open VWorks software. Wait for the program to finish loading. Press the login button at the top and enter the account information.

- 3. Lift the hood sash until it is just aligned with the red arrows. Turn on the light and the fan. Turn on the switch on the right side of the Bravo and wait for a steady blue indicator light.
- 4. Before placing any items inside, wipe down the hood and the Bravo deck with RNase or DNA Away.
- 5. Open the PBAL VWorks form: File > Open and select:  
C:\VWorksWorkspace\NGS\Forms\PBAL.VWForm. To be able to see the form you must change the file type to “all types” at the bottom right of the window.
- 6. Ensure that the 96 LT head is on the Bravo. Otherwise, refer to the SOP: *EGL006\_Changing heads on the Agilent Bravo*.
- 7. In the VWorks form, from the ‘select protocol’ drop down menu choose: “Bisulphite Bead Clean Up”. Enter the number of rows of samples to be processed and protocol-specific parameters:

Bead = 2 uL

DNA = 37.5 uL

Binding buffer = 180 uL

Desulphonation buffer = 60 uL

Elute = 15 uL

- 8. Place all needed items on the Bravo deck in their appropriate locations:

Positions 1-3: new 96-well tip boxes

Position 4: coolrack+ 96 well plate \("Binding + Beads")

Position 5: low volume magnet \Magnum FLX

Position 6: 96 well plate containing bisulfite treated DNA \("sc-PBAL DNA").

Position 7: empty

Position 8: new 96 well deep-well reservoir \(1 or 2mL)

Position 9: Axygen HP reservoir for 80% ethanol \Deep one

- 9. Make sure to check if everything is positioned correctly and to remove all covers before starting of the program.
- 10. At the bottom of the form, hit the Start button. The Bravo will initialize.
- 11. If an error about a plate being detected in the gripper pops up, hit 'Ignore'. Another error about W axis will pop up shortly thereafter. Hit 'Retry'. The Bravo should now begin the protocol.
- 12. Before any tasks begin, VWorks will ask you to configure the tip state editor. Pause the protocol, and go to Tools > Tip State Editor.
- 13. Click the '...' button on the right of the tip box name and change the tip state as necessary to match the tip box on the deck. Repeat for all tip boxes, and then hit 'OK', then 'Continue'.
- 14. The program will add the DNA to the beads \Pos6àPos4 and aliquot the ethanol \Pos9àPos8:
  - 14.1. Bravo will retrieve tips from the tip box at Pos3 and transfer the DNA from the "sc-PBAL DNA" plate at Pos6 to the 'Binding + Beads' plate at Pos4 and mix. The tips will then be returned to Pos3.
  - 14.2. Bravo will retrieve tips from the tip box at Pos2 and aliquot ethanol from reservoir \pos9 into ethanol plate \pos8. You will need to pause the program when the tips are hovering above Pos9 to pour the fresh 80% ethanol into the reservoir. After Bravo aliquot ethanol, the tips will then be

returned to Pos2. Pause the program and cover the ethanol plate at Pos8 right after Bravo drop all the tips into tip box to prevent evaporation.

*Note: The evaporation in the BSC is very intense and the ethanol concentration is critical to DNA recovery. Thus, the ethanol cannot be without a cover for any extended period of time.*

- 15. Bravo will retrieve tips from the tip box at Pos3 and mix the 'Beads + Binding' plate at Pos4 again. The tips will then be returned to Pos3. Wait until the tips are returned before covering the 'Beads + Binding' plate.
- 16. Bravo will then incubate the DNA with the beads for another 8 minutes \ (total 10 min).
- 17. After incubation, Bravo will prompt you to move the 'Beads + Binding' plate from Pos4 to the magnet at Pos5.
- 17.1. Before clicking 'Continue', place the plate on the magnet at Pos5 and incubate for two minutes \ (set a timer).
- 17.2. Click 'Continue' and the Bravo will incubate the plate on the magnet for 3.5 minutes set.

*Note: This solution is very viscous and this additional time is necessary to allow all of the beads to settle on the magnet. This will help ensure we recover as much DNA as possible.*

- 18. Next, Bravo will prompt you to remove the reservoir from the Pos9 and replace it with a 96 well deep-well reservoir \ (Waste), and to remove the DNA plate from Pos6 and replace it with the UV-treated Desulphonation buffer plate.
- 19. Next, Bravo will remove the binding and lysis buffer from DNA Plate \ (Pos5):
  - 19.1. Bravo will retrieve tips from the tip box at Pos3 and remove all of the liquid from the DNA plate \ ('Binding + Beads' plate) at Pos5. Pause the protocol when Bravo hovers above Pos5 and

uncover the plate. The tips will then be returned to Pos3.

*Note: Be sure to check that all of the liquid has been aspirated as the ethanol percentage is critical in the subsequent steps.*

- 20. Next, Bravo will perform two 80% ethanol washes and add desulphonation buffer:
  - 20.1. Bravo will retrieve tips from the tip box at Pos2 and then aspirate 80% ethanol from Pos8. Pause the protocol when the Bravo machine hovers above Pos8 to remove the cover on the ethanol plate \Pos8).
  - 20.2. The ethanol will be gently dispensed into the DNA plate \Pos5).
  - 20.3. Bravo will let the ethanol solution and the beads incubate for 30 seconds before aspirating all of the liquid from the wells \Pos5) and dispensing the waste fluid at Pos9.
  - 20.4. Bravo will then perform a second identical ethanol wash.
  - 20.5. After the waste from the 2<sup>nd</sup> ethanol wash is dispensed at Pos9, pause the protocol when the Bravo hovers above the desulphonation plate \Pos6). Remove the desulphonation plate cover \Pos6) and cover the ethanol plate \Pos8).
  - 20.6. Bravo will retrieve 60uL of desulphonation buffer from Pos6 and dispense it into the DNA plate at Pos5. The tips will then be returned to Pos2.
- 21. Bravo will incubate the DNA with the desulphonation buffer for 15 minutes. Cover the DNA plate \Pos5).
- 22. After the 15 minutes incubation, Bravo will prompt with a pop-up message. Follow the instructions and remove the plate cover on Pos5 before clicking 'Continue'.
- 23. Bravo will discard the waste fluid and perform two ethanol washes:
  - 23.1. Bravo will retrieve tips from the tip box at Pos2 and then aspirate the used desulphonation buffer from Pos5 and discard the waste fluid at Pos9.

- 23.2. Bravo will then aspirate 80% ethanol from Pos8 to perform the first wash. Pause the protocol when the Bravo machine hovers above Pos8 to remove the cover on the ethanol plate \Pos8.
- 23.3. The ethanol will be gently dispensed onto the DNA plate \Pos5.
- 23.4. Bravo will let the ethanol solution and the beads incubate for 30 seconds before aspirating all of the liquid from the wells \Pos5 and dispensing the waste fluid at Pos9.
- 23.5. Bravo will then perform a second identical ethanol wash.
- 23.6. After the waste from the 2<sup>nd</sup> ethanol wash is discarded, let the DNA plate dry for one minute uncovered \start a timer for one minute). The tips will then be returned to Pos2.
- 23.7. Cover the DNA plate \Pos5 when the timer alarm goes off and let the DNA dry \covered for two additional minutes.
- 24. While the beads are drying, replace the plate at Pos6 with your UV-treated QEB plate.
- 25. After two minutes, Bravo will prompt you with a pop-up message. Remove the cover on the QEB plate \Pos6 before clicking 'Continue'.
- 26. Bravo will then add 15uL of QEB \Pos6 to your DNA plate \Pos4:
  - 26.1. Bravo will retrieve tips from the tip box at Pos1 and aspirate 15uL of QEB from Pos6.
  - 26.2. Pause the protocol when the Bravo hovers above Pos4 to dispense the QEB. Remove the cover from the DNA plate and move the plate from Pos5àPos4.
  - 26.3. Bravo will dispense the QEB into the DNA plate at Pos4 and mix to resuspend the beads.
- 27. After the beads are re-suspended in EB buffer, cover the plate with a BioRad PCR cover and place the plate in the Eppendorf thermomixer at 56°C for 15 minutes at 2000 rpm \according to pop-up message). Tape the plate down to the incubator to prevent the plate from flying off.
- 27.1. Set a timer for five minutes and when the alarm goes off, briefly turn the thermomixer down to 1700 rpm to allow the liquid near to the top of the vortex to reincorporate into the larger volume. Then turn the thermomixer back up to 2000 rpm.
- 27.2. Set another timer for five minutes and repeat.

- 28. While the plate is incubating start preparation for 1<sup>st</sup> DNA synthesis.

## 8. sc 1<sup>st</sup> DNA Synthesis

- 1. Retrieve reagents needed for 1<sup>st</sup> DNA synthesis \ (except enzymes) from -20° C freezer, thaw them and place them on ice.
- 2. Working on ice, prepare the DNA denaturation mix according to the following calculator:
- 3. Mix the pre-denaturation mix very well by repeated pulse-vortexing, spin down in a minifuge, and keep it on ice.
- 4. Aliquot 72uL of the mix into one 12-well strip tube \((7.25 uL\*\*8rows+14uLdead volume=72uL).
- 5. Change the tip box at position 2 on Bravo.
- 6. Pause the program and update the tip editor with Box-position2.
- 7. Place the master mix strip-tube on row A of a chilled cool-rack at position 7 on Bravo.
- 8. Aliquot 7.25uL of pre-denaturation mix into each will of a new LoBind plate. Place this plate on a chilled cool-rack at position 6 on Bravo.
- 9. After the 56°C incubation is complete, place the “Binding + Beads” plate in a thermocycler and close the hot lid. Keep it in for 5 seconds to remove any condensation on the tape pad. If there is any droplet on the side of the wells, spin the plate down shortly for 3~4 sec.
- 10. Place the “Binding + Beads” plate back on the Bravo deck: on top of the magnet in position 5.

- 11. The robot will first aliquot the master mix brew from the 12-well strip tube into the new LoBind plate 7.25 uL/well at position 6. Then it will transfer the elute DNA 15 uL/well into the brew plate and mix.
- 12. After the program completes, seal the plate with BioRad PCR cover and spin down the “scPBAL PR” plate for 1 minute at 4°C at 3000 rpm.
- 13. Incubate the “scPBAL PR” plate at 98°C for 1 minute in a thermocycler and immediately spin down the plate at 3000 rpm for 1 minutes at 4°C. Place this plate on ice, keep it COLD.
- 14. Working on ice, prepare post-denaturation mix according to the following calculator:
- 15. Vortex the buffer before addition to the brew.
- 16. Remove the enzyme from -20°C freezer and place it in the chilled tube coolrack for transport to the PCR workstation.
- 17. Mix the enzyme by flicking the tube, spin down in a minifuge, and place it back in the chilled tube coolrack.
- 18. When you pipette the enzyme, aspirate slowly. After dispensing the enzyme into the brew, wash the tip by pipetting up and down. Place the brew back on ice. Return the enzyme back into the -20°C freezer before proceeding.

- 19. Mix the brew very well by multiple pulse-vortexing and keep it on ice.
- 20. Aliquot 27uL per well of the post-denaturation mix into a row of the “RV” plate. Cover and if necessary spin the plate down at 3000rpm for 1min, 4°C to collect the liquid on the bottom. Place this plate in a -20°C chilled coolracks.
- 21. Place the “scPBAL RP” plate on the other -20°C chilled plate coolrack.
- 22. Using P20 multichannel, add 3uL per well of the post-denaturation mix into each row of the “scPBAL RP” plate. After each row addition, set P20 multichannel to 10uL, mix each row up and down 10 times. Change tips between rows.
- 23. After mixing of the last row, seal the plate with BioRad PCR cover, spin the plate down at 3000 rpm, 4°C for 1min.
- 24. Place the plate in the thermocycler, close the lid and run the program pbat-rand-a:

4°C for 10 minutes

4°C to 37°C ramping at 4°C/minute

37°C for 30 minutes

98°C for 1 minutes

4°C forever

- 25. Place the coolracks back in the -20°C freezer to chill for the next step.

## 9. sc 2<sup>nd</sup> DNA synthesis

- 1. About 15 minutes before the program is finished start preparing for the second round of random priming.
- 2. Working on ice, prepare 2<sup>nd</sup> DNA synthesis mix according to the following calculator:
- 3. All reagents \ (except enzymes) must be pulse-vortexed and spin down in a minifuge before addition to the brew. Enzymes should be added last.
- 4. When ready to add the enzyme, pulse-vortex the brew multiple times, then spin down in a minifuge, and place back on ice.
- 5. Remove the Klenow exo – \ (50U/uL) from -20°C freezer and place it in the chilled tube cool rack for transport to the PCR workstation.
- 6. Mix each enzyme by flicking the tube, then spin down in a minifuge and place it back in the chilled tube cool rack.
- 7. When pipetting the enzyme, aspirate slowly to assure an accurate volume transfer. Enzyme storage buffers contain glycerol, which makes the solution more viscous than water.
- 8. After dispensing the enzyme into the brew, wash the tip by pipetting up and down. After enzyme addition, place the brew immediately back on ice. Return the enzyme back into the -20°C freezer before proceeding.
- 9. Mix the entire 2<sup>nd</sup> DNA synthesis mix very well by multiple pulse-vortexing, spin down in a minifuge and place it back on ice.

- 10. Once the pbat-rand program is finished, immediately spin down the “scPBAL RP” plate for 2 minutes at 4°C at 3000 rpm. Place the plate on ice.
- 11. Aliquot 45uL/well of the prepared mix into row F of “RV” plate. Cover and keep it on ice. If needed, spin down for 1min at 3000 rpm at 4°C. Place this plate in a -20°C chilled coolrack.
- 12. Place the “scPBAL RP” plate on another -20°C chilled coolrack.
- 13. Using a P20 multichannel, add 5 uL per well of the 2<sup>nd</sup> DNA synthesis mix to each row of the “scPBAL RP” plate. After each addition, set the multichannel to 15 uL and mix up and down at least 10X, lifting your pipet when dispensing and aspirating from the bottom of the well. Change tips between rows.
- 14. Seal the plate with a BioRad PCR cover and spin down for 1 minute at 4°C at 3000 rpm.
- 15. Place the plate in the thermocycler, close the lid, and run the program pbat-rand-b:

4°C for 30 seconds

4°C to 37°C ramping at 1°C/15 seconds

37°C for 30 minutes

70°C for 10 minutes

4°C forever

- 16. After the program finishes, spin down the plate at 3000 rpm for 1min at 4°C.
- 17. In hood, change the PCR cover to Aluminum Cover. Seal and label with name and date, and store at -20°C overnight.

***Clean up your workstation. Remove garbage. This concludes Day 1 of this protocol.***

## **DAY 2**

### **10. SeraMag Bead Cleanup \BCU and End Repair/Phosphorylation**

- 1. Pre-chill two coolracks at -20°C. Put on a new disposable lab coat, clean workstation and Bravo.
- 2. Take out 20% PEG SeraMag beads from 4°C \ (6 ml is required for one full 96-well plate). Mix by vortexing and leave them to warm at room temperature for at least 30 minutes.
- 3. Ensure that the correct 96 LT head is on the Bravo.
- 4. Turn on the Bravo computer and open VWorks. Wait for the program to finish loading. Press the login button at the top and enter your account information.
- 5. Lift the hood sash until it is just above the red arrows. Turn on the light and the fan. Turn on the switch on the right side of the Agilent Bravo and wait for a steady blue indicator light.
- 6. Clean the Bravo deck with RNase or DNA Away.
- 7. Prepare 50mL of 70% ethanol \ (mix 35mL of 100% ethanol with 15mL of ultrapure water).
- 8. Pour Qiagen EB buffer into a clean reservoir. Aliquot 100 uL of EB buffer into each well of a new AB1400 plate. Label this plate the “EB” plate.

- 9. Retrieve “scPBAL RP” plate from -20°C. Spin down at 3000 rpm for 1min, 4°C.
- 10. Measure the volume of three random DNA wells \ (should be 30 uL, but may be less due to evaporation) and using P20 multichannel add sufficient EB \ (usually 21-24 uL) to reach 50 uL/well. After each row addition, mix well by pipetting up and down 10X. Change tips between rows.

*Note: It is better to have >50 uL than to have <50 uL in this step.*

- 11. Make sure that the DNA/reaction plate is spun down at 3000rpm for 1min, 4°C before placing it on the Bravo deck.
- 12. Once SeraMag beads reach room temperature, aliquot them into one row of a 450uL Axygen plate.
- 13. Using P200 multichannel, aliquot 55 uL of beads into each well of a new AB1400 plate. Label this plate the “beads”. If there are beads on the side of the well, short spin of 4-5 seconds is allowed. Do not spin down beyond that.
- 14. Open the PBAL form. File > Open and select: C:\VWorks Workspace\NGS\Forms\PBAL.VWForm. To be able to see the form you must change the file type at the bottom right of the window.
- 15. In the form, from the ‘select protocol’ drop down list choose “Ampure XP Bead Cleanup-tony”. Hit the ‘Display Initial Setup’ button on the form.
- 16. Set up the deck on the Bravo deck according to the setup diagram on the screen which should match the image below:

Positions 1-3: New 96-well tip boxes \ (full plate of tips)

Position 4: Coolrack + "DNA" plate \ (make sure the plate is spun down)

Position 5: low volume magnet \ (Magnum FLX)

Position 6: Coolrack + "beads" plate

Position 7: empty

Position 8: 96 well 450V reservoir

Position 9: Axygen LP reservoir for 70% ethanol

- 17. Enter the number of rows to be processed \ (8 for a full plate) and set the variables as follows:

DNA volume = 50 uL

Bead volume = 50 uL

Elution volume = 35 uL

Ethanol volume = 150 uL

- 18. Check the Bravo deck if all of the items are present and placed correctly. Make sure that all of the covers have been removed from plates and tip boxes before proceeding.
- 19. At the bottom of the NGS form, hit the Start button. The Bravo will initialize. If an error about a plate being detected in the gripper pops up, hit 'Ignore'. Another error will pop up shortly thereafter. Hit 'Retry'. The Bravo should now begin the protocol.

- 20. Before any tasks begin, VWorks will ask you to configure the tip state editor. Pause the protocol, and go to Tools > Tip State Editor.
- 21. Click the ‘...’ button on the right of the tip box name and change the tip state to match the tip box on the deck. Repeat for all tip boxes then hit ‘OK’ and ‘Continue’.

Note: While the protocol is being executed watch the Bravo to make sure that all volumes are being correctly pipetted. For example, there should be no empty space in the tips when beads are being added to the DNA.

- 22. The program will add the beads \Pos6 to the DNA plate \Pos4. Bravo will retrieve tips from Pos3 and transfer 50uL of beads from Pos6 to the DNA plate at Pos4 and mix. The tips will then be returned to Pos3.
- 23. After bead addition, during the incubation, pause the protocol and cover the DNA plate with a plastic cover.
- 24. The program will aliquot the ethanol into the 96 well reservoir \Pos9àPos8)
- 24.1. Bravo will retrieve tips from the tip box at Pos2 and aliquot ethanol from the reservoir \Pos9 into the ethanol plate \Pos8). Pause the program when the machine hovers above Pos9 to pour the fresh 70% Ethanol into the reservoir. The tips will be returned to Pos2 after the last of the ethanol is aliquoted.
- 24.2. After ethanol aliquoting, pause the program and cover the ethanol plate at Pos8.
- 25. The program will then incubate the DNA plate with the beads for 8 minutes \10 minutes total).
- 26. After incubation, the program will prompt you to put the plate on the magnet and replace the ethanol reservoir from Pos9 with an empty Axygen 450 waste plate.

- 26.1. Place the plate on the magnet at Pos5 and incubate for 5 minutes.

*Note: Check the walls of the wells to ensure that all of the liquid is at the bottom of the well before placing the plate on the magnet. Spin for 3-4s in the centrifuge if this condition is not met.*

- 27. Next, Bravo will remove the waste fluid from the DNA plate \ (Pos5).
  - 27.1. Bravo will retrieve tips from the tip box at Pos3 and proceed to remove all of the liquid from the DNA plate at Pos5. Pause the protocol when Bravo hovers above Pos5 and uncover the plate.
  - 27.2. Bravo will dispense the waste fluid at Pos9. The tips will then be returned to Pos3.
- 28. Next, Bravo will perform two 70% ethanol washes.
  - 28.1. Bravo will retrieve tips from the tip box at Pos2 and then aspirate 70% ethanol from Pos8. Pause the protocol when the Bravo machine hovers above Pos8 to remove the cover on the ethanol plate \ (Pos8).
  - 28.2. The ethanol will be gently dispensed into the DNA plate \ (Pos5).
  - 28.3. Bravo will let the ethanol solution and the beads incubate for 30 seconds before aspirating all of the liquid from the wells \ (Pos5) and dispensing the waste fluid at Pos9.
  - 28.4. Bravo will then perform a second identical ethanol wash.
  - 28.5. After the waste from the 2<sup>nd</sup> ethanol wash is dispensed at Pos9, set a timer for one minute. The tips will then be returned to Pos2.
- 29. When the timer alarms, cover the plate \ (Pos5) and let the plate dry for two additional minutes.

*Note: Before continuing, inspect the reaction plate to make sure that all of the traces of ethanol are evaporated. The beads should be completely dry but not cracked. Make sure the beads are not over-dried as that reduces DNA recovery.*

- 30. Next, Bravo will prompt you to move the DNA plate from Pos5 to Pos4 and to place the QEB plate at Pos6. Do not move the DNA plate yet, but place the QEB plate at Pos6. Remove the cover on the QEB plate and click 'Continue'.
- 31. The program will then add 35 uL QEB \(Pos6) to the DNA plate \(Pos4) and incubate for a minimum of four minutes.
- 31.1. Bravo will retrieve tips from the tip box at Pos1 and aspirate QEB from Pos6.
- 31.2. Bravo will then dispense the QEB into the DNA plate at Pos4. Pause the protocol when the machine hovers above Pos4. Uncover the DNA plate \(Pos5) and move it to Pos4.
- 31.3. The tips will then be returned to Pos1.
- 31.4. Cover the DNA plate \(Pos4) when the machine is no longer in motion.
- 32. After the EB buffer has been added and mixed with dried beads pause the program and in a 2.0mL tube prepare the End-repair master mix according to the following calculator:
- 33. All reagents \(except enzymes) must be pulse-vortexed and spin down in a minifuge before addition to the brew. Enzymes should be added last. When ready to add the enzymes, pulse-vortex the end repair master mix multiple times, then spin down in a minifuge, and place back on ice.
- 34. Remove the enzymes from -20°C freezer and place them in the chilled tube cool rack for transport to the PCR workstation. Mix each enzyme by flicking the tube, then spin down in a minifuge and place it back in the chilled tube cool rack.
- 35. When pipetting the enzyme, aspirate slowly to assure an accurate volume transfer. Enzyme storage buffers contain glycerol, which makes the solution more viscous than water. After dispensing the enzyme into the brew, wash the tip by pipetting up and down.

*Note: Never double dip into the solution with the same tip.*

- 36. After enzyme addition place the brew immediately back on ice. Return the enzymes back into the -20°C freezer before proceeding.
- 37. Gently pulse-vortex the brew multiple times to assure an even distribution of all of the components. Pulse-vortexing means that you stop vortexing every time a full vortex is formed in the tube. Spin down the brew in a minifuge and immediately place it back on ice.
- 38. Working on ice, aliquot 143 uL of the mix into one 12-well strip tube.
- 39. Change the tip box at position 2 on Bravo and pause the program and update the tip editor with Box-position2.
- 40. Place the master mix strip-tube on row A of a chilled cool-rack at position 7 on Bravo. Place the elution plate back on the Bravo deck: on top of the magnet in Pos5.
- 41. The robot will first aliquot the master mix brew from the 12-well strip tube into the new LoBind plate 15 uL/well at position 6. Bravo will transfer \Pos5 the DNA elution into the brew plate \Pos6 and mix.
- 42. After the program completes, cover the plate and spin down the plate for 1 minute at 4°C at 3000 rpm.
- 43. Incubate at room temperature for 30 minutes then proceed to the next step.

## 11. Bead Cleanup and A-Tailing

- 1. Set up the Bravo exactly as stated in Bead Clean-up step 10 except with the following change in the parameters:

DNA volume = 50 uL

Bead volume = 50 uL

Elution volume = 25 uL

Ethanol volume = 150 uL

- 2. Make sure that the DNA/reaction plate is spun down at 3000rpm for 1min, 4C before placing it on the Bravo deck.
- 3. Aliquot SeraMag beads into one row of a 450uL Axygen plate.
- 4. Using P200 multichannel, aliquot 55 uL of beads into each row of a “beads” plate. If there are beads on the side of the well, short spin of 4-5 seconds is allowed.
- 5. Check the Bravo deck if all of the items are present and placed correctly. Make sure that all of the covers have been removed from plates and tip boxes before proceeding.

- 6. Start the protocol. Before any tasks begin, VWorks will ask you to configure the tip state editor. Pause the protocol, and go to Tools > Tip State Editor.
- 7. Click the '...' button on the right of the tip box name and change the tip state to match the tip box on the deck. Repeat for all tip boxes then hit 'OK' and 'Continue'.

Note: While the protocol is being executed watch the Bravo to make sure that all volumes are being correctly pipetted. For example, there should be no empty space in the tips when beads are being added to the DNA.

- 8. The program will add the beads \((Pos6) to the DNA plate \((Pos4).
- 8.1. Bravo will retrieve tips from Pos3 and transfer 50uL of beads from Pos6 to the DNA plate at Pos4 and mix. The tips will then be returned to Pos3.
- 8.2. Pause the protocol and cover the DNA plate.
- 9. The program will aliquot the ethanol into the 96 well reservoir \((Pos9àPos8)
  - 9.1. Bravo will retrieve tips from the tip box at Pos2 and aliquot ethanol from the reservoir \((Pos9) into the ethanol plate \((Pos8). Pause the program when the machine hovers above Pos9 to pour the fresh 70% Ethanol into the reservoir. The tips will be returned to Pos2 after the last of the ethanol is aliquoted.
  - 9.2. Pause the program and cover the ethanol plate at Pos8.
- 10. The program will then incubate the DNA plate with the beads for 8 minutes \((10 minutes total).
- 11. After incubation, the program will prompt you to put the plate on the magnet and replace the ethanol reservoir from Pos9 with an empty Axygen 450 waste plate.
- 11.1. Place the plate on the magnet at Pos5 and incubate for two minutes \((set a timer).

- 11.2. Click 'Continue' when the timer alarms and incubate for an additional 3.5 minutes.

*Note: Check the walls of the wells to ensure that all of the liquid is at the bottom of the well before placing the plate on the magnet. Spin for 3-4s in the centrifuge if this condition is not met.*

- 12. Next, Bravo will remove the waste fluid from the DNA plate \Pos5).

- 12.1. Bravo will retrieve tips from the tip box at Pos3 and proceed to remove all of the liquid from the DNA plate at Pos5. Pause the protocol when Bravo hovers above Pos5 and uncover the plate.
- 12.2. Bravo will dispense the waste fluid at Pos9. The tips will then be returned to Pos3.
- 13. Next, Bravo will perform two 70% ethanol washes.
- 13.1. Bravo will retrieve tips from the tip box at Pos2 and then aspirate 70% ethanol from Pos8. Pause the protocol when the Bravo machine hovers above Pos8 to remove the cover on the ethanol plate \Pos8).
- 13.2. The ethanol will be gently dispensed into the DNA plate \Pos5).
- 13.3. Bravo will let the ethanol solution and the beads incubate for 30 seconds before aspirating all of the liquid from the wells \Pos5) and dispensing the waste fluid at Pos9.
- 13.4. Bravo will then perform a second identical ethanol wash.
- 13.5. After the waste from the 2<sup>nd</sup> ethanol wash is dispensed at Pos9, set a timer for one minute. The tips will then be returned to Pos2.
- 14. When the timer alarms, cover the plate \Pos5) and let the plate dry for two additional minutes.

*Note: Before continuing, inspect the reaction plate to make sure that all of the traces of ethanol are evaporated. The beads should be completely dry but not cracked. Make sure the beads are not over-dried as that reduces DNA recovery.*

- 15. Next, Bravo will prompt you to move the DNA plate from Pos5 to Pos4 and to place the QEB plate at Pos6. Do not move the DNA plate yet, but place the QEB plate at Pos6. Remove the cover on the QEB plate and click 'Continue'.
- 16. The program will then add 25 uL QEB \Pos6 to the DNA plate \Pos4 and incubate for a minimum of four minutes.
- 16.1. Bravo will retrieve tips from the tip box at Pos1 and aspirate QEB from Pos6.
- 16.2. Bravo will then dispense the QEB into the DNA plate at Pos4. Pause the protocol when the machine hovers above Pos4. Uncover the DNA plate \Pos5 and move it to Pos4.
- 16.3. The tips will then be returned to Pos1.
- 16.4. Cover the DNA plate \Pos4 when the machine is no longer in motion.
- 17. After the EB buffer has been added and mixed with dried beads, in a 1.5mL tube prepare A-addition brew according to the following calculator:
- 18. Aliquot 95 uL of the mix into one 12-well strip tube.
- 19. Change the tip box at position 2 on Bravo. Pause the program and update the tip editor with Box-position2.
- 20. Place the master mix strip-tube on row A of a chilled cool-rack at position 7 on Bravo. Place a LoBind plate on a chilled cool-rack at position 6 on Bravo.
- 21. Place the elution plate back on the Bravo deck: on top of the magnet in position 5.
- 22. The robot will first aliquot the master mix brew from the 12-well strip tube into the new LoBind plate 10 uL/well at position 6. Then it will transfer \Pos5 the elute DNA 25 uL/well into the brew plate \Pos6 and mix.

- 23. After the program completes, seal the plate with a BioRad PCR cover and spin down the “A-addition” plate at 4°C at 3000 rpm for 1 minute.
- 24. Incubate the final reaction (35 uL total volume) at 37°C for 30 minutes and then inactivate at 70°C for 10 minutes.

*Note: Do not cover with the Thermocycler lid. Loosely cover with Thermomixer lid.*

- 25. While waiting, prepare for the next step.

## 12. sc PBAL direct ligation

- 1. Retrieve the 5X Quick Ligation Buffer from -20°C and thaw at room temperature then transfer to ice. Mix very well before use. This reagent contains high concentration of PEG, which makes it more difficult to pipette. Take an extra care to pipette this reagent slowly to assure accuracy of volume transfer.
- 2. Retrieve one plate single use aliquot of 10 uM PE Adapter. Prepare 300uL of 1 uM Adapter (1/10 dilution, 30 uL stock + 270uL EB) by diluting with EB buffer. Aliquot the diluted 1 uM adapter into one row of a 96-well plate, 24uL/well. Cover the plate and keep it on ice.
- 3. Prepare the ligation brew in one 5 mL tube according to the following calculator:

- 4. All reagents \except enzymes must be pulse-vortexed and spin down in a minifuge before addition to the brew. Enzymes should be added last. When ready to add the enzymes, pulse-vortex the end repair master mix multiple times, then spin down in a minifuge, and place back on ice.
- 5. Remove the enzymes from -20°C freezer and place them in the chilled tube cool rack for transport to the PCR workstation. Mix each enzyme by flicking the tube, then spin down in a minifuge and place it back in the chilled tube cool rack.
- 6. When pipetting the enzyme, aspirate slowly to assure an accurate volume transfer. Enzyme storage buffers contain glycerol, which makes the solution more viscous than water.
- 7. After dispensing the enzyme into the brew, wash the tip by pipetting up and down. Do not double dip with the same tip into a stock solution. After enzyme addition, place the brew immediately back on ice.
- 8. Return the enzymes back into the -20°C freezer before proceeding.
- 9. Gently pulse vortex the brew multiple times to assure an even distribution of all of the components. Pulse vortexing means that you stop vortexing every time a full vortex is formed in the tube. Briefly spin down the brew in a minifuge and place it back on ice.
- 10. Aliquot 200 uL of the mix into one 12-well strip tube.
- 11. Change the tip box at position 2 on Bravo. Pause the program and update the tip editor with Box-position2.
- 12. Place the master mix strip-tube on row A of a chilled cool-rack at position 7 on Bravo.

- 13. Place the elution plate back on the Bravo deck: on top of the magnet in position 5.
- 14. Manually add 2 uL adaptor from the reservoir row to each well of new LoBind plate using P20 multichannel pipette. Label the plate “PBAL Ligation”. Place the plate on a chilled cool-rack at position 6 on Bravo.
- 15. The robot will first aliquot the master mix brew from the 12-well strip tube into the new LoBind plate 23 uL/well at position 6. Click ‘Continue’ and Bravo will transfer \Pos5) the DNA elution 35 uL/well into the brew plate \Pos6) and mix.
- 16. Once the program finishes, cover the ‘PBAL Ligation’ plate at Pos6 and move it to the laminar flow hood. Add 23 uL of the ligation master mix into each well via P200 multichannel pipette.
- 17. Use the P200 multichannel pipette to mix. Set the pipette to 40 uL and then aspirate the reaction mixture from the bottom of each well and slightly lift the tip of the pipette before dispensing on the top. Repeat this ten times to ensure thorough mixing.

Note: Pipet slowly to avoid bubbles.

- 18. Cover the plate with an aluminum cover, and spin down at 3000rpm for 1min at 4C.
- 19. Incubate the “PBAL Ligation” plate at room temperature overnight. Label the date and sample name clearly.
- 20. Clean up your single cell PCR work-station and Bravo. Turn off all of the used equipment.

- 21. Enter all of the data in your laboratory notebook. This concludes Day 2 of this protocol.

**Clean up your workstation. Remove garbage. This concludes Day 2 of this protocol.**

## DAY 3

### 13. 1<sup>st</sup> Bead Cleanup After Ligation

- 1. Take out 20% PEG SeraMag beads from 4°C (enough for one full 96-well beads clean-up will be 6 tubes), mix by vortexing and leave them to warm at room temperature for at least 30 minutes. Before proceeding make sure that the SeraMag bead solution fully reached room temperature. Using a cold solution results in reduced DNA recovery.
- 2. Aliquot 55 uL of beads into each well of a new plate. Label this plate the “beads” plate. Do NOT use a reservoir for this step as the beads will settle and the PEG concentration will not be consistent.
- 3. Aliquot 120 uL of EB buffer into each well of a new plate. Label this plate the “EB” plate.
- 4. Set up the bravo exactly as stated in Bead-Cleanup and End-Repair (step 10) except with the following parameters:

DNA volume = 60 uL

Bead volume = 48 uL

Elution volume = 50 uL

- 5. The program will add the beads \Pos{6} to the DNA plate \Pos{4}.
  - 5.1. Bravo will retrieve tips from Pos3 and transfer 50uL of beads from Pos6 to the DNA plate at Pos4 and mix. The tips will then be returned to Pos3.
  - 5.2. Pause the protocol and cover the DNA plate.
  
- 6. The program will aliquot the ethanol into the 96 well reservoir \Pos{9à8}
  - 6.1. Bravo will retrieve tips from the tip box at Pos2 and aliquot ethanol from the reservoir \Pos{9} into the ethanol plate \Pos{8}. Pause the program when the machine hovers above Pos9 to pour the fresh 70% Ethanol into the reservoir. The tips will be returned to Pos2 after the last of the ethanol is aliquoted.
  - 6.2. Pause the program and cover the ethanol plate at Pos8.
  
- 7. The program will then incubate the DNA plate with the beads for 8 minutes \Pos{10} (10 minutes total).
  
- 8. After incubation, the program will prompt you to put the plate on the magnet and replace the ethanol reservoir from Pos9 with an empty Axygen 450 waste plate.
  
- 8.1. Place the plate on the magnet at Pos5 and incubate for two minutes \Pos{11} (set a timer).
- 8.2. Click 'Continue' when the timer alarms and incubate for an additional 3.5 minutes.

*Note: Check the walls of the wells to ensure that all of the liquid is at the bottom of the well before placing the plate on the magnet. Spin for 3-4s in the centrifuge if this condition is not met.*

- 9. Next, Bravo will remove the waste fluid from the DNA plate \Pos{5}.
  - 9.1. Bravo will retrieve tips from the tip box at Pos3 and proceed to remove all of the liquid from the DNA plate at Pos5. Pause the protocol when Bravo hovers above Pos5 and uncover the plate.
  - 9.2. Bravo will dispense the waste fluid at Pos9. The tips will then be returned to Pos3.
- 10. Next, Bravo will perform two 70% ethanol washes.

- 10.1. Bravo will retrieve tips from the tip box at Pos2 and then aspirate 70% ethanol from Pos8. Pause the protocol when the Bravo machine hovers above Pos8 to remove the cover on the ethanol plate \Pos8.
  - 10.2. The ethanol will be gently dispensed into the DNA plate \Pos5.
  - 10.3. Bravo will let the ethanol solution and the beads incubate for 30 seconds before aspirating all of the liquid from the wells \Pos5 and dispensing the waste fluid at Pos9.
  - 10.4. Bravo will then perform a second identical ethanol wash.
  - 10.5. After the waste from the 2<sup>nd</sup> ethanol wash is dispensed at Pos9, set a timer for one minute. The tips will then be returned to Pos2.
- 11. When the timer alarms, cover the plate \Pos5 and let the plate dry for two additional minutes.

*Note: Before continuing, inspect the reaction plate to make sure that all of the traces of ethanol are evaporated. The beads should be completely dry but not cracked. Make sure the beads are not over-dried as that reduces DNA recovery.*

- 12. Next, Bravo will prompt you to move the DNA plate from Pos5 to Pos4 and to place the QEB plate at Pos6. Do not move the DNA plate yet, but place the QEB plate at Pos6. Remove the cover on the QEB plate and click 'Continue'.
  - 13. The program will then add 50 uL QEB \Pos6 to the DNA plate \Pos4 and incubate for a minimum of four minutes.
  - 13.1. Bravo will retrieve tips from the tip box at Pos1 and aspirate QEB from Pos6.
  - 13.2. Bravo will then dispense the QEB into the DNA plate at Pos4. Pause the protocol when the machine hovers above Pos4. Uncover the DNA plate \Pos5 and move it to Pos4.
  - 13.3. The tips will then be returned to Pos1.
  - 13.4. Cover the DNA plate \Pos4 when the machine is no longer in motion.
- 14. Place a new LoBind plate at Pos6. Bravo should elute the supernatant directly into new plate.

- 15. Take the final eluted product and use it as the input DNA for the next step.

#### **14. 2<sup>nd</sup> Bead cleanup after ligation and PCR amplification of library**

- 1. Aliquot 55 uL of beads into each well of the “beads” plate. Do NOT use a reservoir for this step as the beads will settle and the PEG concentration will not be consistent.
- 2. Set up the Bravo exactly as stated in Bead-Cleanup and End-Repair \ (step 10) except with the following parameters:

DNA volume = 50 uL

Bead volume = 50 uL

Elution volume = 25 uL

- 3. Start the protocol. Replace the “beads” plate with the “EB” plate after the beads have been added to the DNA plate.
- 4. The program will add the beads \ (Pos6) to the DNA plate \ (Pos4).
  - 4.1. Bravo will retrieve tips from Pos3 and transfer 50uL of beads from Pos6 to the DNA plate at Pos4 and mix. The tips will then be returned to Pos3.
  - 4.2. Pause the protocol and cover the DNA plate.
- 5. The program will aliquot the ethanol into the 96 well reservoir \ (Pos9àPos8)
- 5.1. Bravo will retrieve tips from the tip box at Pos2 and aliquot ethanol from the reservoir \ (Pos9) into the ethanol plate \ (Pos8). Pause the program when the machine hovers above Pos9 to pour the fresh 70% Ethanol into the reservoir. The tips will be returned to Pos2 after the last of the ethanol is aliquoted.

- 5.2. Pause the program and cover the ethanol plate at Pos8.
- 6. The program will then incubate the DNA plate with the beads for 8 minutes \ (10 minutes total).\
- 7. After incubation, the program will prompt you to put the plate on the magnet and replace the ethanol reservoir from Pos9 with an empty Axygen 450 waste plate.
- 7.1. Place the plate on the magnet at Pos5 and incubate for two minutes \ (set a timer).
- 7.2. Click 'Continue' when the timer alarms and incubate for an additional 3.5 minutes.

*Note: Check the walls of the wells to ensure that all of the liquid is at the bottom of the well before placing the plate on the magnet. Spin for 3-4s in the centrifuge if this condition is not met.*

- 8. Next, Bravo will remove the waste fluid from the DNA plate \ (Pos5).
- 8.1. Bravo will retrieve tips from the tip box at Pos3 and proceed to remove all of the liquid from the DNA plate at Pos5. Pause the protocol when Bravo hovers above Pos5 and uncover the plate.
- 8.2. Bravo will dispense the waste fluid at Pos9. The tips will then be returned to Pos3.
- 9. Next, Bravo will perform two 70% ethanol washes.
- 9.1. Bravo will retrieve tips from the tip box at Pos2 and then aspirate 70% ethanol from Pos8. Pause the protocol when the Bravo machine hovers above Pos8 to remove the cover on the ethanol plate \ (Pos8).
- 9.2. The ethanol will be gently dispensed into the DNA plate \ (Pos5).
- 9.3. Bravo will let the ethanol solution and the beads incubate for 30 seconds before aspirating all of the liquid from the wells \ (Pos5) and dispensing the waste fluid at Pos9.
- 9.4. Bravo will then perform a second identical ethanol wash.

- 9.5. After the waste from the 2<sup>nd</sup> ethanol wash is dispensed at Pos9, set a timer for one minute. The tips will then be returned to Pos2.
- 10. When the timer alarms, cover the plate \ (Pos5) and let the plate dry for two additional minutes.

Note: Before continuing, inspect the reaction plate to make sure that all of the traces of ethanol are evaporated. The beads should be completely dry but not cracked. Make sure the beads are not over-dried as that reduces DNA recovery.

- 11. Next, Bravo will prompt you to move the DNA plate from Pos5 to Pos4 and to place the QEB plate at Pos6. Do not move the DNA plate yet, but place the QEB plate at Pos6. Remove the cover on the QEB plate and click 'Continue'.
- 12. The program will then add 25 uL QEB \ (Pos6) to the DNA plate \ (Pos4) and incubate for a minimum of four minutes.
  - 12.1. Bravo will retrieve tips from the tip box at Pos1 and aspirate QEB from Pos6.
  - 12.2. Bravo will then dispense the QEB into the DNA plate at Pos4. Pause the protocol when the machine hovers above Pos4. Uncover the DNA plate \ (Pos5) and move it to Pos4.
  - 12.3. The tips will then be returned to Pos1.
  - 12.4. Cover the DNA plate \ (Pos4) when the machine is no longer in motion.
- 13. While waiting for the protocol, prepare the PCR mastermix in a tube and aliquot into one row of a new 96-well plate. Label this the "reservoir" plate.
- 14. Prepare the PCR brew in a 5 mL tube according to the following calculator:
- 15. Aliquot 211 uL of the mix into one 12-well strip tube.
- 16. Change the tip box at position 2 on Bravo. Pause the program and update the tip editor with Box-position2.
- 17. Place the master mix strip-tube on row A of a chilled cool-rack at position 7 on Bravo.

- 18. Place a LoBind plate on a chilled cool-rack at position 6 on Bravo.
- 19. Place the elution plate back on the Bravo deck: on top of the magnet in position 5.
- 20. The robot will first aliquot the master mix brew from the 12-well strip tube into the new LoBind plate 23 uL/well at position 6. Then it will transfer \Pos5 the elute DNA 25 uL/well into the brew plate \Pos6 and mix.
- 21. Using a P20 multichannel pipette, manually add 2 uL of the index primer from the Indexing Primer plate to each reaction. Label this plate “PCR.”
- 22. Spin down the plate at 3000rpm, 4C, for 2min.
- 23. Incubate the “PCR” plate in the thermocycler using the program pcr-gsc using 7 cycles. Check the cycle number and setting before starting PCR.

pcr-gsc program:

98°C for 1 minute

98°C for 30 seconds

65°C for 15 seconds

70°C for 15 seconds

70°C for 5 minutes

4°C forever

## 15. Bead cleanup after PCR

- 1. Aliquot 50 uL of beads into each well of the “beads” plate. Do NOT use a reservoir for this step as the beads will settle and the PEG concentration will not be consistent.
- 2. Set up the bravo exactly as stated in Bead-Cleanup and End-Repair \ (step 7) except with the following parameters:

DNA volume = 50 uL

Bead volume = 45 uL

Elution volume = 27 uL

- 3. The program will add the beads \ (Pos6) to the DNA plate \ (Pos4).
- 3.1. Bravo will retrieve tips from Pos3 and transfer 50uL of beads from Pos6 to the DNA plate at Pos4 and mix. The tips will then be returned to Pos3.
- 3.2. Pause the protocol and cover the DNA plate.
- 4. The program will aliquot the ethanol into the 96 well reservoir \ (Pos9àPos8)
- 4.1. Bravo will retrieve tips from the tip box at Pos2 and aliquot ethanol from the reservoir \ (Pos9) into the ethanol plate \ (Pos8). Pause the program when the machine hovers above Pos9 to pour the fresh 70% Ethanol into the reservoir. The tips will be returned to Pos2 after the last of the ethanol is aliquoted.
- 4.2. Pause the program and cover the ethanol plate at Pos8.
- 5. The program will then incubate the DNA plate with the beads for 8 minutes \ (10 minutes total).

- 6. After incubation, the program will prompt you to put the plate on the magnet and replace the ethanol reservoir from Pos9 with an empty Axygen 450 waste plate.
- 6.1. Place the plate on the magnet at Pos5 and incubate for two minutes \set a timer).
- 6.2. Click 'Continue' when the timer alarms and incubate for an additional 3.5 minutes.

***Note:** Check the walls of the wells to ensure that all of the liquid is at the bottom of the well before placing the plate on the magnet. Spin for 3-4s in the centrifuge if this condition is not met.*

- 7. Next, Bravo will remove the waste fluid from the DNA plate \Pos5).
- 7.1. Bravo will retrieve tips from the tip box at Pos3 and proceed to remove all of the liquid from the DNA plate at Pos5. Pause the protocol when Bravo hovers above Pos5 and uncover the plate.
- 7.2. Bravo will dispense the waste fluid at Pos9. The tips will then be returned to Pos3.
- 8. Next, Bravo will perform two 70% ethanol washes.
- 8.1. Bravo will retrieve tips from the tip box at Pos2 and then aspirate 70% ethanol from Pos8. Pause the protocol when the Bravo machine hovers above Pos8 to remove the cover on the ethanol plate \Pos8).
- 8.2. The ethanol will be gently dispensed into the DNA plate \Pos5).
- 8.3. Bravo will let the ethanol solution and the beads incubate for 30 seconds before aspirating all of the liquid from the wells \Pos5) and dispensing the waste fluid at Pos9.
- 8.4. Bravo will then perform a second identical ethanol wash.
- 8.5. After the waste from the 2<sup>nd</sup> ethanol wash is dispensed at Pos9, set a timer for one minute. The tips will then be returned to Pos2.
- 9. When the timer alarms, cover the plate \Pos5) and let the plate dry for two additional minutes.

Note: Before continuing, inspect the reaction plate to make sure that all of the traces of ethanol are evaporated. The beads should be completely dry but not cracked. Make sure the beads are not over-dried as that reduces DNA recovery.

- 10. Next, Bravo will prompt you to move the DNA plate from Pos5 to Pos4 and to place the QEB plate at Pos6. Do not move the DNA plate yet, but place the QEB plate at Pos6. Remove the cover on the QEB plate and click 'Continue'.
- 11. The program will then add 27 uL QEB \((Pos6) to the DNA plate \((Pos4) and incubate for a minimum of four minutes.
- 11.1. Bravo will retrieve tips from the tip box at Pos1 and aspirate QEB from Pos6.
- 11.2. Bravo will then dispense the QEB into the DNA plate at Pos4. Pause the protocol when the machine hovers above Pos4. Uncover the DNA plate \((Pos5) and move it to Pos4.
- 11.3. The tips will then be returned to Pos1.
- 11.4. While the DNA is eluting, cover the DNA plate \((Pos4) when the machine is no longer in motion.
- 11.5. After the incubation for the DNA elution is over, spin the plate for 10-20 seconds in plate centrifuge.
- 11.6. Place the plate on the magnet \((Pos5) and uncover the plate.
- 12. Place a new \((labelled) LoBind plate at Pos6. Bravo should elute the supernatant directly into new plate.
- 13. Cover the plate with a plastic cover, spin down at 2000g for 1min, 4°C. Proceed to the next step or seal with an aluminum cover and store at -20°C.

## 16. qPCR QC

- 1. Work at post-PCR bench. Perform all work on ice.
- 2. Place a 384 well coolrack in -20°C freezer to chill. Get fresh ice.
- 3. Turn on ViiA7 and it's computer. Open the program ViiA 7 1.2.
- 4. Wipe down and turn on Bravo. Make sure it is **96ST** head. Load VWorks as described previously. Choose program: *PBAL-qPCR pro*.
- 5. Label a clean 96 well plate as a “reservoir”. Prepare two 1.5ml amber vials for qPCR brew on ice. Label one as “target”, the other one as “library”.
- 6. Prepare the brews according to the following calculators.
- 7. Aliquot 76 uL/well of the target brew into one row of reservoir plate, label the row “target”.
- 8. Aliquot 76 uL/well of the library brew into second row of reservoir plate, label the row “library”.
- 9. Retrieve qPCR-384 well plate. Mark A1 at A1 corner. Mark on the left of wells the rows for target reactions, use quadrant A. Mark on the right of the wells the rows for library reactions, use quadrant 4.
- 10. Working on ice, aliquot 9 uL of brew into each well as defined from reservoir.
- 11. Add negative qPCR control wells \ (9 uL of brew) manually to the bottom right corner of the plate.

- 11.1. Negative control for target: O22 and O24
- 11.2. Negative control for library: P21 and P23.
- 12. Cover the qPCR plate and keep it on ice. Keep the plate protected from light.
- 13. Pour EB buffer \ (post-PCR) into a reservoir and using P200 multichannel aliquot 100uL/well into a 96 well plate and cover with a plastic seal.
- 14. Set up Bravo deck as per image below:

Position 1: empty 384 tip box

Position 2: empty

Position 3: new box of 384 tip box

Position 4: coolrack + DNA sample plate

Position 5: chilled coolrack + 384 qPCR plate with brew

Position 6: coolrack + EB buffer plate

Position 7, 8, 9, empty

- 15. Click “Run protocol”. VWorks will prompt you to configure the tip state editor.
- 16. Select Pause, click on Tools, then Tip State Editor. Click “...” button on the right of the tip box name and adjust the tip state to match the tip boxes on the Bravo deck. Repeat for all tip boxes.

Hit Continue and start the Bravo process.

- 17. The Bravo will add the DNA into the target wells and dilute the DNA 1:100 in EB buffer before transferring into library wells.

- 18. After Bravo program is done remove the plate from the Bravo deck.
- 19. Seal the plate very well with a MicroAmp optical qPCR cover. Use the MicroAmp Adhesive Film Applicator to create a good seal, especially on the perimeter of the plate.
- 20. Spin the plate down at 3000 rpm, for 1 min, at 4°C. Place the plate inside the ViiA7 instrument.  
Make sure that A1-well matches the A1 position on the tray.

- 21. In the ViiA 7 software click “New experiment”. Set up plate. After set up save it as template file \*\*.edt for later use.

Target will be quadrant 1, and Library will be quadrant 4. \ (e.g. figure below)

Negative control for target: O22 and O24

Negative control for library: P21 and P23

- 22. After set up the template, check that the cycle settings are correct:

98°C for 1min

98°C for 15 sec

60°C for 30 sec

72°C for 30 sec

- 23. The reaction volume should be 10uL and the passive reference should be set to none.
- 24. Save qPCR run to your folder, name it with plate label and date.
- 25. Hit “Run” button, the qPCR will start. Leave qPCR running overnight or if possible, wait for the qPCR results. If you wait for the qPCR, complete the pooling and ethanol precipitation step so it can be incubated at -20°C for overnight.

- 26. Clean up your workstation. Remove garbage. This concludes Day 3 of this protocol.

## DAY 4

### 17. qPCR Analysis, sample pooling and precipitation

- 1. Analyze qPCR data using *qPCR pipeline.Rmd* following instructions.
  - 1.1. instructions:

# 1. Change the title to desired file name

# 2. Select the correct excel file \ (press tab between quotes, choose from the list)

# 3. Make sure the wells are defined \ (positive, negative, tencell,hundredcell)

# 4. Set cutoff to be between 8-10

# 5. Press "Knit HTML"

# 6. View the plot, if needed, adjust cut off value slightly

# 7. Press "Knit HTML" again

# 8. Check through figures, save/print results and confirm correct file names

# 9. Upload to JIRA, under the appropriate library construction ticket

\\"\\\"

- 1.2. Define a cutoff for success

Successful passed samples will cluster well in plot figure, the cutoff should be set right above the clustered plots. For example:

- 1.3. Check that there are no systematic errors with the plate

- 2. Percentage of passed samples should be above 75-80%. Check that the average CT values of the passed wells is consistent with previous sample plates \ (Target and Library).

Note: Average CT value for Target should be between 21-23, average CT value for Library should be between 13-15. Delta CT between Target\_Ct and Library\_Ct should be between 6-9.

- 3. Working on ice, pool all of the passed wells and negative controls together into a 2mL tube. Exclude failed wells and positive controls \ (usually G1 or as marked).

- 4. Measure the total volume and, working on ice, set up ethanol precipitation as follows:

X \ (volume pooled in uL)

0.1\*X of 3M Sodium Acetate pH 5.5 \ (in uL)

- 5. Mix well by pulse-vortexing. Add 1.3 uL mussel glycogen \ (marked as MG, 20mg/mL) and mix well by pulse-vortexing.

- 6. Calculate the total volume and add 2.5X\ (total volume in uL) of cold 100% ethanol. Vortex thoroughly. It is important that the solution is very well mixed. Split the volume across multiple 1.5mL tubes.

- 7. Incubate precipitations at -20°C for at least 2 hour but overnight is preferred.

- 8. While waiting, pre-chill the centrifuge to 4°C.

- 9. After -20°C incubation, place all tubes in the same orientation in the pre-chilled to 4°C centrifuge.

- 10. Spin down at 15,000g \ (max rpm) at 4°C, for 40 min.

- 11. Prepare fresh 70% ethanol using ultrapure water. Take out and aliquot of 20% PEG SeraMag beads to warm up to room temperature for at least 30 min.

*Note: The following steps must be performed on ice.*

- 12. After centrifugation visually locate the pellet. Carefully discard the supernatant while avoiding the DNA pellet.
- 13. Add 1mL of 70% ethanol, plate the tube inside the centrifuge in the same orientation as before, and spin down at 15000g \ (max rpm) at 4°C, for 4 min.
- 14. After centrifugation visually locate the pellet and carefully aspirate the supernatant.
- 15. Spin down the tube in minifuge to collect all of the ethanol on the bottom. With P10 remove the final traces of ethanol.
- 16. Dry the pellet at room temperature until the pellet becomes translucent \ (maximum 5 minutes).  
Keep a close eye on the pellets so that they do not over-dry.
- 17. When the pellet becomes clear, resuspend the DNA in each tube with 20 uL of room temperature EB buffer. Mix up and down with the pipette.
- 18. After the pellets are fully dissolved, pool all volume into one tube. Measure the volume and top up with EB buffer to a multiple of 50uL. For example, if the volume is 80uL add an additional 20uL of EB buffer to a total volume 100uL \ (which is 2X 50uL).

## 18. Library pool purification using SeraMag beads

- 1. Make sure that the 20% SeraMag beads have fully reached room temperature before proceeding and use freshly made \ (on the same day) 70% ethanol.
- 2. Working at post PCR work station, using a single channel P100, aliquot the pooled and precipitated single cell PCR library products - 50uL per well into one row of a new LoBind plate.
- 3. Mix the 20% SeraMag beads very well and aliquot 55ul per well into one row of a reservoir plate \ (corresponding to the number of DNA wells). Using P200 multichannel, to each 50uL of DNA add 45uL of room temperature 20%PEG SeraMag beads \ (0.9X ratio) and immediately mix by pipetting up and down at least 10X.
- 4. Incubate at room temperature for 10 min.
- 5. After 10min incubation move the plate to the magnet and incubate for 3 min. Make sure that all of the beads are separated to the sides and the solution is completely clear before proceeding.
- 6. Keep the plate on the magnet for the next few steps.
- 7. Without disturbing the beads, using a single channel P200, carefully remove the clear supernatant. Make sure not to remove any beads.
- 8. On the magnet, using multichannel P200, add 150ul of 70% ethanol and incubate for 30 seconds.
- 9. From each well, carefully aspirate the ethanol using single channel P200.

- 10. Using multichannel P200, add 150uL 70% ethanol and incubate for 30 seconds.
- 11. From each well, using single channel P200 set to 170uL, carefully remove all of the ethanol.
- 12. After the second wash keep the plate still on the magnet. Using P10 aspirate the remaining traces of ethanol from the bottom of each well. Make sure not to remove any beads,
- 13. Let the beads dry at room temperature for 2 min. Do not over-dry the beads. You should not see any cracks.
- 14. When the beads are dry, remove the plate from the magnet. Using P20, add 15uL of EB buffer and mix very well by pipetting up and down. Make sure that all of the beads are re-suspended. The solution should be uniformly brown.
- 15. Incubate at room temperature for 3min.
- 16. After 3min elution, place the plate back onto the magnet and incubate for 1 min. Make sure that all of the beads are pulled to the sides and the solution is completely clear.
- 17. After 1min incubation, using P20 carefully transfer the supernatant \ (containing the eluted DNA) into a new 1.5 mL tube. Label the tube with sample/pool ID.
- 18. Use 1uL of the sample for Qubit assay and run another 1uL on HS Agilent to observe the fragment distribution. Expected yield should be > 1 ng/uL. Average size of the final product should be around 300bp.

- 19. Store the sample at -20C until ready for sequencing. Record all of the data in your notebook.
- 20. Clean up your workstation. Remove garbage. This concludes Day 4 of this protocol.

## Figures

	01	02	03	04	05	06	07	08	09	10	11	12	13	14	15	16	17	18	19	20	21	22	23	24
A																								
B																								
C																								
D																								
E																								
F																								
G																								
H																								
I																								
J																								
K																								
L																								
M																								
N																								
O																								
P																								

single cell  
10 cells

Figure 1

Sorting plate layout (Step 3.1)

scPBAL Lysis buffer calculator					
number of reactions	96	extra brew (%)	30		
		Per reaction (per # of reactions)	dead volume	total volume (uL)	
100 mM Tris HCl pH 7.5	0.4	38.4	12.0	50.4 ( )	100 mM Tris HCl pH 7.5
10% SDS	0.8	76.8	24.0	100.8 ( )	10% SDS
20 mg/ml Protease K	0.2	19.2	6.0	25.2 ( )	20 mg/ml Protease K
EB buffer	2.6	249.6	78.0	327.6 ( )	EB buffer
total volume (uL)	4.0			504.0      42.00	

Figure 2

Lysis Brew Table

scPBAL silica beads calculator					
number of reactions	96	Per reaction ( per # of reactions)	dead volume ( μL)	total volume ( μL)	
extra brew (%)	20				
Silica beads		2	192	38	230

Figure 3

Silica beads calculator

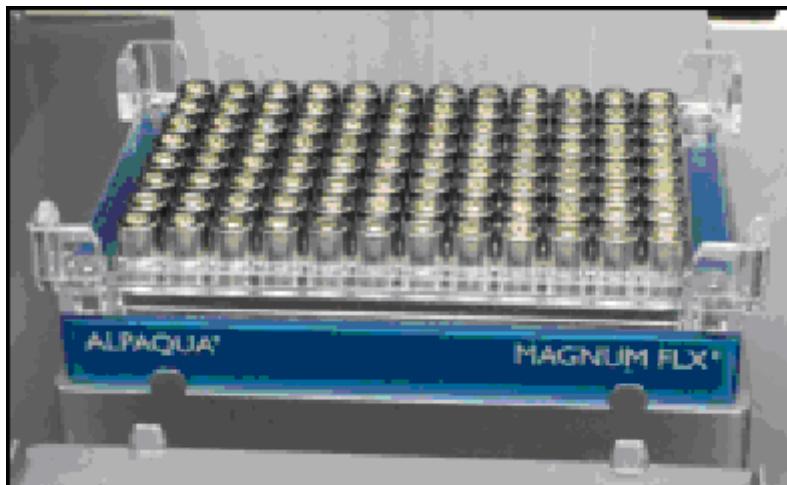


Figure 4

Magnum FLX magnet