

Functional improvement and satisfaction with a wearable hip exoskeleton in community- living adults

Jihye Kim

Department of Physical and Rehabilitation Medicine, Center for Prevention and Rehabilitation, Heart Vascular Stroke Institute, Samsung Medical Center, Sungkyunkwan University School of Medicine, Seoul

Hyelim Chun

Department of Physical and Rehabilitation Medicine, Center for Prevention and Rehabilitation, Heart Vascular Stroke Institute, Samsung Medical Center, Sungkyunkwan University School of Medicine, Seoul

Su-Hyun Lee

Department of Physical and Rehabilitation Medicine, Center for Prevention and Rehabilitation, Heart Vascular Stroke Institute, Samsung Medical Center, Sungkyunkwan University School of Medicine, Seoul

Hwang-Jae Lee

Robot Business Team, Samsung Electronics, Suwon

Yun-Hee Kim (✉ yun1225.kim@samsung.com)

Department of Physical and Rehabilitation Medicine, Center for Prevention and Rehabilitation, Heart Vascular Stroke Institute, Samsung Medical Center, Sungkyunkwan University School of Medicine, Seoul

Research Article

Keywords: exoskeleton device, gait, robot, personal satisfaction, physical fitness

Posted Date: April 25th, 2022

DOI: <https://doi.org/10.21203/rs.3.rs-1567172/v1>

License:   This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

Abstract

Background: Demand for wearable devices and supportive technology is growing as these devices have the potential to enhance physical function and quality of life in users. The purpose of this study was to investigate usability and satisfaction after performing functional and gait exercise with a wearable hip exoskeleton in community-living adults.

Methods: Two-hundred and twenty-five adults (mean age 67.52 ± 10.99) residing in the local community participated in this study. All participants (middle-aged group, $n=75$; old-aged group, $n=150$) performed 40-minutes of exercise once with a wearable hip exoskeleton in various environments. The EX1 (Samsung Electronics Co., Ltd., Suwon, Republic of Korea), which functions as a wearable hip exoskeleton, was used. Physical function was assessed before and after exercise with the EX1 using the 10-meter walking test (10MWT), four square step test (FSST), timed up and go test (TUG), 6-minute walking test (6MWT), and short physical performance battery (SPPB). In addition, after completing exercise with the EX1, the usability and satisfaction questionnaires were evaluated.

Results: Gait speed, TUG, and FSST showed statistically significant improvements after exercise with the EX1 in both groups ($p < 0.05$). In 6MWT, a significant increase was observed in the middle-aged group ($p < 0.05$) but not in the old-aged group. In SPPB, there was a significant improvement in the old-aged group ($p < 0.05$) but not in the middle-aged group. On the other hand, positive results in usability and satisfaction were noticed in both groups. In preference between resistance and assist mode of the EX1, the old-aged group preferred the assist mode and the middle-aged group preferred the resistance mode.

Conclusion: These results demonstrate that a single session of exercise with the EX1 was effective in improving physical performance of both middle- and old-aged adults, with positive feedback from most of the participants.

Trial registration: Clinical trials registration information: ClinicalTrials.gov Identifier: NCT05106881 (03/11/2021).

Background

Physical activity, which is associated with quality of life, decreases with age due to loss of muscle mass and strength [1], cardiac and respiratory disease [2], and other factors. Decreased physical activity during the aging process leads to metabolic disorders and other chronic diseases, such as cancer, diabetes, and cerebrovascular and cardiovascular diseases [3]. Regular physical activity such as walking, cycling, dancing, and running leads to positive physiological changes. Regular physical activity improves autonomic balance, bone density, capillary density, muscle fiber size, neuromuscular coordination, stroke volume, blood coagulation, and inflammation [4]. Moreover, these physiological changes result in decreased depression, weight gain, fractures, injurious falls, osteoporosis, and mortality, as well as increased physical and cognitive function [4]. A previous study reported that regular physical activity could increase the life expectancy of the world's population by 0.68 years [5].

Walking is one of the easiest regular physical activities. Walking is the cheapest and easiest activity for health promotion and consumes larger amounts of energy than other daily sports activities. Gait function refers to the mobility required for daily life performance, which can predict clinical conditions in various aspects [6]. In previous studies, inactive adults experienced 3–8% muscle loss over 10 years with decreased metabolic rate and fat accumulation during rest [7], but walking exercise improved walking economy and functionality [8], muscle size and quality [9], functional balance, and reaction time [10], which are related to gait quality.

Recently, functional exercise has been carried out under various conditions, such as applying a load, using props, or combining various conditions. Resistance gait exercise enhances balance and gait parameters [11] and decreases the fear of falling [12]. A previous study showed that, after resistance gait exercise using an underwater treadmill, gait parameters including step length, velocity, and cadence were significantly increased [13]. In addition, an assistive therapeutic exercise program is effective in improving preferred gait speed [14].

Robot technology in the healthcare field is being actively used in clinical practice as it has been developed in the surgical and rehabilitation medical fields. However, in recent years, the technological advances in daily assistive robots have gone beyond their limited use for patients in the medical field [15]. Wearable exoskeletons are being actively developed to assist and strengthen physical functions for not only disabled, but also non-disabled people. A wearable exoskeleton helps to improve gait by assisting with voluntary movement of the lower extremity joints during gait [16, 17]. Furthermore, gait exercise with a wearable hip exoskeleton improves cardiopulmonary function. In a previous study, gait training with an assisted-exoskeleton robot required less oxygen consumption than a home exercise program of self-paced overground walking without a robot at the same speed in the elderly [18].

The EX1, developed by Samsung Electronics (Suwon, Republic of Korea), is a personalized robot with a light weight of 2.1kg that is worn on the hip joints. In our previous study in the elderly, there were statistically significant improvements in gait speed, excessive muscle activity, respiration, and metabolic energy during gait with EX1 compared to walking without it [16].

Demand for wearable devices and supportive technology is growing because these devices have potential to enhance physical functions and quality of life of users. Furthermore, among the factors to be considered when using a wearable robot, user stability and fit are important. Previous studies on EX1 investigated the effect on physical function rather than usability and satisfaction with the wearable robot. Thus, wearable devices need to be evaluated by actual users in terms of wearability [19]. This study was designed to investigate the usability, satisfaction, and physical function from a single session of functional and gait exercise with the EX1 in community-living, middle- and old-aged adults.

Methods

The participants were recruited from local community residents who use silver town or welfare centers. Two-hundred and twenty-five adults who met the following inclusion criteria were enrolled in this study:

no history of central nervous system disease and age between 40 and 84 years. Subjects with uncontrolled severe high blood pressure or diabetes, history of uncontrolled cardiovascular disease, severe dizziness that might lead to a fall, and cognitive disorders that hinder the ability to understand or comply with study instructions were excluded. General characteristics of the subjects are summarized in Table 1. The study protocol was approved by the Institutional Review Board of Samsung Medical Center, Seoul, Korea (No. 2021-04-058), and informed consent was provided by all subjects before participating in the study.

Experimental protocol

This study protocol was designed as a single group, and all participants performed a single session of exercise with EX1. All participants received 40 minutes of exercise with the EX1: 20 minutes of functional exercise including sit-to-stand and balance exercise and 20 minutes of gait exercise including stair climbing and over-ground and incline walking with the assist and resistance modes of EX1. To confirm the effect of a single session of exercise with EX1, physical functions measured by the 10-meter walking test (10MWT), timed up and go test (TUG), four square step test (FSST), 6-minute walking test (6MWT), and short physical performance battery (SPPB) were evaluated before and after the exercise program. All outcome measures were performed without the EX1. After completing a single session of exercise with the EX1, the usability and satisfaction questionnaire for EX1 were evaluated (Fig 1).

Wearable hip exoskeleton (EX1)

The EX1, which was developed by Samsung Electronics, is a minimized exoskeleton worn on the hip joints. It is very lightweight and user-customizable, weighing about 2.1 kg (Fig 2). EX1 can provide assistive or resistive torque forces around both hip joints for both extension and flexion direction during gait as needed, and it promotes physical function in daily life. EX1 consists of a pair of actuators that generate force on the left and right hip joints, a hip brace on the waist, a pair of thigh frames, and a thigh belt [20].

Measurement tools

Physical function evaluation

To measure physical function, 10MWT, TUG, FSST, 6MWT, and SPPB were performed. 10MWT is the most effective method for predicting falls and evaluating gait ability by measuring gait speed, and it has high test-retest reliability in healthy adults (ICC=0.93-0.91) [21]. For measurement, subjects were asked to walk a total of 15 m at a comfortable speed. The time it took to walk 10 m was measured, excluding the initial 2.5 m acceleration and the final 2.5 m deceleration, and the result in seconds was converted into speed (m/s). Measurements were repeated twice, and the average value was used.

To evaluate the dynamic balance ability among physical functions, TUG and FSST were measured. The TUG test is used as a standard test method in clinical practice as a representative test method for measuring gait ability as well as dynamic balance ability of elderly and brain injury patients, and it has

high intra- and inter-tester reliability (ICC) in the elderly (ICC=.92-.99) [22]. The FSST test is a method of evaluating dynamic balance and movement ability. It measures the time it takes to walk forward, backward, and sideways over a low obstacle as fast as subjects can, and it has high test-retest reliability (ICC=0.87) [23].

To evaluate walking endurance, 6MWT was measured. 6MWT is a representative method for measuring gait aerobics and endurance in the elderly and patients with cardiopulmonary disease. To measure gait endurance, subjects are asked to walk a set trajectory for 6 minutes, and the total walking distance is measured. It has excellent test-retest reliability for the elderly (ICC=0.95) [22].

SPPB is a test that consists of walking speed, sit-to-stand on a chair, and balance tests. It has been used as a predictive tool for dysfunction and can be helpful in functional monitoring in the elderly. The score ranges from a minimum of 0 points to a maximum of 12 points. SPPB has been shown to have validity as a predictor of fall risk and mortality and has excellent test-retest reliability for the elderly (ICC=0.91) [24].

The usability and satisfaction questionnaire

As there was no appropriate usability and satisfaction questionnaire for evaluating the wearable hip exoskeleton, the questionnaire was developed and applied through previous research [17] and consultation with experts (Table 2). A questionnaire was developed by setting usability and satisfaction evaluation areas. The safety questionnaire is one of the most important parts to determine whether EX1 can be used safely. The operability question is a factor to realize the function of the gait robot. The questionnaire includes operational convenience, effectiveness, and efficiency.

Data preprocessing and statistical analysis

All data were analyzed with SPSS version 22.0 program (IBM, Armonk, NY, USA). Results were calculated as mean and standard deviation values. Statistical significance levels for all measurements were set as $p < 0.05$.

Physical function evaluation, usability, and satisfaction tests were analyzed by dividing the age into two subgroups: a middle-aged group 40 to 64 years old and an old-aged group 65 to 84 years old. To evaluate the feasibility of a single session with the EX1, paired t-tests were used to compare outcome measures between pre- and post-exercise.

To evaluate the usability and satisfaction questionnaire, frequency analysis was used. In addition, the usability and satisfaction tests with standardized β coefficients in linear regression analysis were used to investigate the relationship between physical function and questionnaire.

Results

Physical Function

In 10MWT, TUG, and FSST, significant increases after a single exercise session with EX1 were observed in both groups ($p < 0.05$) (Fig 3). In 6MWT, there was a statistically significant improvement only in the middle-aged group ($p < 0.05$). In SPPB, there was a significant improvement in the old-aged group ($p < 0.05$) but not in the middle-aged group.

Usability and satisfaction of the EX1

In the safety domain (involving items such as risk of falls and control of risk factors), after using the EX1, positive responses were confirmed in both groups. The responses were mostly positive in the satisfaction domain, but there were some items with difference by age group. The middle-aged group showed more positive responses than the old-aged group in the easiness of use, usefulness, and perception of the EX1. In addition, the middle-aged group showed more positive responses than the old-aged group in the questionnaire on whether the assist and resist mode of the EX1 help with gait exercises. Though the old-aged group tended to prefer the assist mode, the middle-aged group tended to prefer the resistance mode of the EX1 (Fig 4).

Regression analysis between general characteristics, usability, and satisfaction

As a result of regression analysis of 128 cases with a combination of 16 dependent variables and 8 independent variables, there were 15 significant results ($Y = aX + b$) (Table 2). The dependent variable (Y) consisted of a total of 16 items related to safety (4 items) and satisfaction (12 items), and the independent variable (X) consisted of a total of 8 items: age, gender, height, weight, body mass index (BMI), health status (2 items; health conditions, level of activity), and experience of fall.

The younger is the user, the easier they tend to think the EX1 was to use, they tend to think that the assist mode of the EX1 helps most with gait, and they tend to be willing to continue using the EX1. If the users think they have better health conditions, they tend to think the EX1 was easy to use. If the user is more active, they think that they control the risk posed by the EX1 (Supplementary 1).

Regression analysis between usability, satisfaction, and physical function

As a result of regression analysis of 240 cases by combining 10 dependent variables and 24 independent variables, there were 25 significant results ($Y = aX + b$) (Table 2). The dependent variable (Y) consisted of a total of 10 items regarding functional evaluation baseline (5 items) and difference of functional evaluation between baseline and after single-session exercise with EX1 (5 items). The independent variable (X) consisted of a total of 24 items related to age, gender, height, weight, body mass index (BMI), health status (2 items; health condition, level of activity), experience of fall, safety (4 items), and satisfaction (12 items).

If the users thought they have better health conditions, they tended to have faster FSST and TUG. If the users considered themselves active, they tended to have faster gait speed, and walk farther in 6 minutes. If the users had experience of falling, they tended to have lower SPPB, slower gait speed, and walk less in 6 minutes; after gait exercise with EX1 these users tended to have higher SPPB than before exercise.

If the users thought there was no risk of falling when they were turning or leaning forward while wearing the robot, after gait exercise with EX1, they tended to have lower SPPB. If the users thought the robot was easy to use, they tend to have higher SPPB, and faster TUG; after gait exercise with EX1 these users tended to have faster FSST than before exercise (Supplementary 2).

Discussion

Our study demonstrates that a single session of exercise with the EX1 improved physical functions. In addition, positive results of the EX1 were confirmed by conducting a usability and satisfaction survey after exercise with EX1.

In this study, statistically significant improvements in gait speed, balance ability, and gait endurance were confirmed through a single session of exercise with the EX1. The results of this study suggest that a single session of exercise with the EX1 has several key advantages for physical function and efficiency. Functional exercise that is effective for improving gait function includes gait exercise at various speeds and directions, treadmill gait, and stair climbing. In addition, the resistance and assistance of the EX1 can be adjusted based on individual physical ability. Therefore, it improves physical function gradually by controlling the intensity and duration of the exercise.

To determine gait quality, we used objective, sensitive, and powerful measurement tools that measure gait performance, dynamic balance ability, and gait endurance [25]. In our study, there was a statistically significant improvement in gait speed. Previous studies have shown that lower gait speed is associated with age, education, and particularly modifiable factors such as impairment of activities of daily life, physical inactivity, and cardiovascular disease [26]. Gait speed is a clinical indicator related to survival rate and predicts functional ability in the elderly [27]. In a previous study, it was reported that gait speed increased by 0.1 m/s as the survival rate increased [28]. These results indicate the importance of staying active and healthy for middle- and old-aged people.

Balance ability, an essential factor in gait ability, is the ability to maintain balance against numerical movement and external stimuli, which reduces muscle weakness due to decreased physical activity and is highly associated with risk of fall due to dynamic balance ability during gait [29, 30]. Physical changes due to aging lead to a decrease in gait function by reducing balance, and it is highly related to the incidence of injuries in the elderly [31]. In our study, a statistically significant improvement was shown in dynamic balance ability through a single session of exercise with the EX1. Falling is a serious problem that threatens the health of the elderly and can lead to premature death due to physical damage, psychological dysfunction, and onset of various diseases [32]. Preventing falls and improving body function require planned and consistent exercise. Decreased physical activity leads to muscle strength weakness, which causes reduced balance ability. Balance training is an essential element in an exercise program because it is highly correlated with risk of falls according to dynamic balance ability while walking.

Gait endurance is also one of the major factors influencing risk of falls in the elderly. It is known that the weaker is the walking endurance, the higher is the likelihood of a fall in the elderly. In our study, endurance improved immediately after a single session of exercise with the EX1 in both age groups, but a significant result was found only in the middle-aged group. Endurance is increased through long-term gait training [33], but in our study, time was insufficient to derive significant results with a single session of exercise with the EX1. However, although it was not significant after single session of exercise, walking distance for 6 minutes improved, indicating the potential for positive results with long-term exercise.

SPPB is a fast and useful measurement tool for predicting falls [34]. In our study, SPPB improved immediately in the old-aged group after a single session of exercise with the EX1, but no significant result was shown due to the ceiling effect in the middle-aged group.

This study was performed to confirm the usability and satisfaction of the EX1. Considering user physical condition and environment, it was divided into user questionnaire evaluation and user function evaluation, and the safety, operability, and satisfaction of the EX1 were evaluated. If an expert or designer conducts a usability evaluation while listening to users' opinions, it is possible to understand the user's needs, inconveniences, strengths, and expectations in a complex way. Regression analysis showed a difference in the experience feedback for the EX1 by age or physical function. However, there were no implications for usability, perceptions, or satisfaction with general characteristics other than age.

As the results of the questionnaire including usability and satisfaction, both middle- and old-aged groups had positive experience feedback for the EX1. Among them, more positive results were shown in the middle-aged group than the old-aged group in a few items. We think that these results were caused by middle-aged people being more open-minded and faster to learn new technologies than the elderly. In the questionnaire, both assist and resistance modes of the EX1 helped with gait, with strongly positive answers in the middle-aged group compared to the old-aged group. In addition, in a questionnaire on the preference between assist and resistance modes of the EX1, the old-aged group preferred assist mode, but the middle-aged group preferred resistance mode. These results indicated that the elderly, who have a decline in gait ability, prefer gait assist, but middle-aged people who need gait training prefer the resist mode of the EX1.

In regression analysis between general characteristics and questionnaire, users tended to think that using the EX1 would have no negative social perceptions if they thought they had lower health conditions. Younger users tend to have positive opinions of the EX1. Although there might be perceptions that exercise using robots is applied only to patients or the elderly [35, 36], this study confirmed that healthy people had positive perceptions of exercise with robots. Therefore, we think that the EX1 can provide a meaningful exercise program not only for the elderly, but also for young people. In regression analysis between questionnaire and physical function, people who experienced a fall within 6 months had better balance ability and physical function after a single session of exercise with the EX1. It was confirmed that the higher was the satisfaction with the function of the robot, the better were the physical endurance

and dynamic balance. We think that such exercise will bring positive results when applied to people with reduced balance ability, which is a risk factor for falls.

We designed this study as a short-term functional and satisfaction evaluation of the EX1. In addition, this study was conducted only with healthy subjects. Thus, usability and satisfaction of the EX1 with subjects with declined physical function and long-term use must be addressed in further studies.

Conclusion

This study demonstrated that a single session of exercise with the EX1 in middle- and old-age persons improved physical performance, including gait and balance, and received positive feedback. A newly developed wearable hip exoskeleton, the EX1, is a potentially useful exercise device for improving gait and physical function not only in the elderly, but also in middle-aged people.

Abbreviations

10MWT: 10-meter walking test

TUG: Timed up and go

FSST: Four square step test

6MWT: 6-minute walking test

SPPB: Short physical performance battery

Declarations

Ethics approval and consent to participate

All participants recruited through Samsung Medical Center provided informed consent before participating in the present study. This study protocol was approved by the ethics committee of the Samsung Medical Center Institutional Review Board.

Consent for publication

Not applicable

Availability of data and material

The datasets supporting the conclusions of this article are included within the manuscript.

Competing interests

The authors declare that they have no competing interests to disclose.

Funding

This study was supported by Samsung Electronics (PH00219391).

Authors' contributions

JHK and HLC contributed to the experimental design, experimental progress, data collecting, data analysis, and drafting of the manuscript. SHL contributed to the experimental design, data analysis, data interpretation, and revising of the manuscript. HJL and YHK contributed to the experimental design, interpreting data, and revising the manuscript. All authors have read and approved the final manuscript.

Acknowledgements

Not applicable

Authors' information

¹Department of Physical and Rehabilitation Medicine, Center for Prevention and Rehabilitation, Heart Vascular Stroke Institute, Samsung Medical Center, Sungkyunkwan University School of Medicine, Seoul, Republic of Korea. ²Robot Business Team, Samsung Electronics, Suwon, Republic of Korea. ³Department of Health Science and Technology, Department of Medical Device Management and Research, Department of Digital Health, SAIHST, Sungkyunkwan University, Seoul, Republic of Korea

References

1. Milanovic Z, Pantelic S, Trajkovic N, Sporis G, Kostic R, James N: **Age-related decrease in physical activity and functional fitness among elderly men and women.** *Clin Interv Aging* 2013, **8**:549–556.
2. Verghese J, LeValley A, Hall CB, Katz MJ, Ambrose AF, Lipton RB: **Epidemiology of gait disorders in community-residing older adults.** *J Am Geriatr Soc* 2006, **54**(2):255–261.
3. Suryadinata RV, Wirjatmadi B, Adriani M, Lorensia A: **Effect of age and weight on physical activity.** *J Public Health Res* 2020, **9**(2):1840.
4. Powell KE, Paluch AE, Blair SN: **Physical activity for health: What kind? How much? How intense? On top of what?** *Annu Rev Public Health* 2011, **32**:349–365.
5. Lee IM, Shiroma EJ, Lobelo F, Puska P, Blair SN, Katzmarzyk PT, Lancet Physical Activity Series Working G: **Effect of physical inactivity on major non-communicable diseases worldwide: an analysis of burden of disease and life expectancy.** *Lancet* 2012, **380**(9838):219–229.
6. Kim J, Lee HJ, Lee SH, Lee J, Chang WH, Ryu GH, Kim YH: **Correlation between cardiopulmonary metabolic energy cost and lower-limb muscle activity during inclined treadmill gait in older adults.** *BMC Geriatr* 2021, **21**(1):469.
7. Westcott WL: **Resistance training is medicine: effects of strength training on health.** *Curr Sports Med Rep* 2012, **11**(4):209–216.

8. Gomenuka NA, Oliveira HB, da Silva ES, Passos-Monteiro E, da Rosa RG, Carvalho AR, Costa RR, Rodriguez Paz MC, Pellegrini B, Peyre-Tartaruga LA: **Nordic walking training in elderly, a randomized clinical trial. Part II: Biomechanical and metabolic adaptations.** Sports Med Open 2020, **6**(1):3.
9. Yoshiko A, Tomita A, Ando R, Ogawa M, Kondo S, Saito A, Tanaka NI, Koike T, Oshida Y, Akima H: **Effects of 10-week walking and walking with home-based resistance training on muscle quality, muscle size, and physical functional tests in healthy older individuals.** Eur Rev Aging Phys Act 2018, **15**:13.
10. Rooks DS, Kiel DP, Parsons C, Hayes WC: **Self-paced resistance training and walking exercise in community-dwelling older adults: effects on neuromotor performance.** J Gerontol A Biol Sci Med Sci 1997, **52**(3):M161-168.
11. Keating CJ, Cabrera-Linares JC, Parraga-Montilla JA, Latorre-Roman PA, Del Castillo RM, Garcia-Pinillos F: **Influence of Resistance Training on Gait & Balance Parameters in Older Adults: A Systematic Review.** Int J Environ Res Public Health 2021, **18**(4).
12. Wollesen B, Mattes K, Schulz S, Bischoff LL, Seydell L, Bell JW, von Duvillard SP: **Effects of Dual-Task Management and Resistance Training on Gait Performance in Older Individuals: A Randomized Controlled Trial.** Front Aging Neurosci 2017, **9**:415.
13. Kim MK, Lee SA: **Underwater treadmill training and gait ability in the normal adult.** J Phys Ther Sci 2017, **29**(1):67–69.
14. Lim J, Lim JY: **Responsiveness of gait speed to physical exercise interventions in at-risk older adults: a systematic review and meta-analysis.** Annals of Geriatric Medicine and Research 2017, **21**(1):17–23.
15. Lee H: **The change of medical environment & wellness view in the era of the 4th industrial revolution.** J Korean Soc Wellness 2017, **12**:215–223.
16. Lee HJ, Lee S, Chang WH, Seo K, Shim Y, Choi BO, Ryu GH, Kim YH: **A Wearable Hip Assist Robot Can Improve Gait Function and Cardiopulmonary Metabolic Efficiency in Elderly Adults.** IEEE Trans Neural Syst Rehabil Eng 2017, **25**(9):1549–1557.
17. Kwon SH, Lee BS, Lee HJ, Kim EJ, Lee JA, Yang SP, Kim TY, Pak HR, Kim HK, Kim HY *et al*: **Energy Efficiency and Patient Satisfaction of Gait With Knee-Ankle-Foot Orthosis and Robot (ReWalk)-Assisted Gait in Patients With Spinal Cord Injury.** Ann Rehabil Med 2020, **44**(2):131–141.
18. Martini E, Crea S, Parri A, Bastiani L, Faraguna U, McKinney Z, Molino-Lova R, Pratali L, Vitiello N: **Gait training using a robotic hip exoskeleton improves metabolic gait efficiency in the elderly.** Sci Rep 2019, **9**(1):7157.
19. Chae UR, Kim K, Choi J, Hyun DJ, Yun J, Lee GH, Hyun YG, Lee J, Chung M: **Systematic usability evaluation on two harnesses for a wearable chairless exoskeleton.** International Journal of Industrial Ergonomics 2021, **84**:103162.
20. Lee HJ, Lee SH, Seo K, Lee M, Chang WH, Choi BO, Ryu GH, Kim YH: **Training for Walking Efficiency With a Wearable Hip-Assist Robot in Patients With Stroke: A Pilot Randomized Controlled Trial.** Stroke 2019, **50**(12):3545–3552.

21. Bohannon RW: **Comfortable and maximum walking speed of adults aged 20–79 years: reference values and determinants.** *Age Ageing* 1997, **26**(1):15–19.
22. Steffen TM, Hacker TA, Mollinger L: **Age- and gender-related test performance in community-dwelling elderly people: Six-Minute Walk Test, Berg Balance Scale, Timed Up & Go Test, and gait speeds.** *Phys Ther* 2002, **82**(2):128–137.
23. Gomez JF, Curcio CL, Alvarado B, Zunzunegui MV, Guralnik J: **Validity and reliability of the Short Physical Performance Battery (SPPB): a pilot study on mobility in the Colombian Andes.** *Colomb Med (Cali)* 2013, **44**(3):165–171.
24. Olsen CF, Bergland A: **"Reliability of the Norwegian version of the short physical performance battery in older people with and without dementia".** *BMC Geriatr* 2017, **17**(1):124.
25. Bortone I, Sardone R, Lampignano L, Castellana F, Zupo R, Lozupone M, Moretti B, Giannelli G, Panza F: **How gait influences frailty models and health-related outcomes in clinical-based and population-based studies: a systematic review.** *J Cachexia Sarcopenia Muscle* 2021, **12**(2):274–297.
26. Busch Tde A, Duarte YA, Pires Nunes D, Lebrao ML, Satya Naslavsky M, dos Santos Rodrigues A, Amaro E, Jr.: **Factors associated with lower gait speed among the elderly living in a developing country: a cross-sectional population-based study.** *BMC Geriatr* 2015, **15**:35.
27. Van Abbema R, De Greef M, Craje C, Krijnen W, Hobbelen H, Van Der Schans C: **What type, or combination of exercise can improve preferred gait speed in older adults? A meta-analysis.** *BMC Geriatr* 2015, **15**:72.
28. Studenski S, Perera S, Patel K, Rosano C, Faulkner K, Inzitari M, Brach J, Chandler J, Cawthon P, Connor EB *et al*: **Gait speed and survival in older adults.** *JAMA* 2011, **305**(1):50–58.
29. Osoba MY, Rao AK, Agrawal SK, Lalwani AK: **Balance and gait in the elderly: A contemporary review.** *Laryngoscope Investig Otolaryngol* 2019, **4**(1):143–153.
30. Gill-Body KM, Hedman LD, Plummer L, Wolf L, Hanke T, Quinn L, Riley N, Kaufman R, Verma A, Quiben M *et al*: **Movement System Diagnoses for Balance Dysfunction: Recommendations From the Academy of Neurologic Physical Therapy's Movement System Task Force.** *Phys Ther* 2021, **101**(9).
31. Gusi N, Carmelo Adsuar J, Corzo H, Del Pozo-Cruz B, Olivares PR, Parraca JA: **Balance training reduces fear of falling and improves dynamic balance and isometric strength in institutionalised older people: a randomised trial.** *J Physiother* 2012, **58**(2):97–104.
32. Jaul E, Barron J: **Age-Related Diseases and Clinical and Public Health Implications for the 85 Years Old and Over Population.** *Front Public Health* 2017, **5**:335.
33. Wang RY, Wang YL, Cheng FY, Chao YH, Chen CL, Yang YR: **Effects of combined exercise on gait variability in community-dwelling older adults.** *Age (Dordr)* 2015, **37**(3):9780.
34. Welch SA, Ward RE, Beauchamp MK, Leveille SG, Trivison T, Bean JF: **The Short Physical Performance Battery (SPPB): A Quick and Useful Tool for Fall Risk Stratification Among Older Primary Care Patients.** *J Am Med Dir Assoc* 2021, **22**(8):1646–1651.
35. Kim Y-H: **Robotic assisted rehabilitation therapy for enhancing gait and motor function after stroke.** *Precision and Future Medicine* 2019, **3**(3):103–115.

Tables

Table 1. General characteristics of participants

Characteristics	Total (<i>N</i> =225)	Middle-aged (<i>n</i> =75)	Old-aged (<i>n</i> =150)
Gender (male / female)	80 / 145	31 / 44	49 / 101
Age (year)	67.52 (10.99) ^a	74.31 (4.79)	53.96 (6.30)
Height (cm)	161.53 (8.26)	159.85 (8.85)	164.88 (7.32)
Weight (kg)	61.76 (10.58)	59.93 (9.32)	65.43 (11.98)
BMI (kg/m ²)	23.59 (3.06)	23.42 (2.92)	23.94 (3.33)
MMSE-K	28.16 (1.82)	27.95 (1.93)	28.57 (1.49)
GDS-15	3.71 (3.32)	4.1 (3.43)	2.93 (2.99)
FES-K	99.32 (3.30)	99.07 (3.92)	99.81 (1.24)
EQ-5D	0.90 (0.08)	0.89 (0.92)	0.93 (0.46)

Note. ^aMean (SD), middle-aged group = 40–64 years, old-aged group = 65–84 years; BMI=Body mass index; MMSE-K=Mini-mental state examination-Korean; GDS-15=Geriatric depression scale-15; FES-K=Fall efficacy scale-Korean; EQ-5D= EuroQol-5 dimension.

Table 2. The usability and satisfaction questionnaire of the EX1

Domain	No.	Item	Strongly disagree	Disagree	Neutral	Agree	Strongly agree
Safety	1	Did you have any risk of falling when turning or leaning forward while using the EX1?	<input type="checkbox"/>				
Safety	2	Did you have a risk of fall or injury while using the EX1?	<input type="checkbox"/>				
Safety	3	Do you think you can control the risks posed by EX1 yourself?	<input type="checkbox"/>				
Safety	4	Did you fear falling while walking with the EX1?	<input type="checkbox"/>				
Satisfaction	1	Was the EX1 easy to use?	<input type="checkbox"/>				
Satisfaction	2	Do you think people with healthy people can also use the EX1?	<input type="checkbox"/>				
Satisfaction	3	Were you not shamed for using EX1?	<input type="checkbox"/>				
Satisfaction	4	Do you think the EX1 will have negative social perceptions?	<input type="checkbox"/>				
Satisfaction	5	Was the weight of the EX1 appropriate for walking?	<input type="checkbox"/>				
Satisfaction	6	Was the EX1 comfortable to wear?	<input type="checkbox"/>				
Satisfaction	7	Were you satisfied with the material of the EX1?	<input type="checkbox"/>				
Satisfaction	8	Do you think the assist mode of the EX1 helps with gait?	<input type="checkbox"/>				
Satisfaction	9	Do you think the resistance mode of the EX1 helps with gait exercises?	<input type="checkbox"/>				
Satisfaction	10	Was there any disturbance caused by noise when using the EX1?	<input type="checkbox"/>				

Domain	No.	Item	Strongly disagree	Disagree	Neutral	Agree	Strongly agree
Satisfaction	11	Are you satisfied with the color and design of the EX1?	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Satisfaction	12	Are you willing to continue using the EX1?	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Satisfaction	13	Between assist and resistance modes of EX1, which was more helpful?	<input type="radio"/> Resistance mode		<input type="radio"/> Assist mode		

Figures

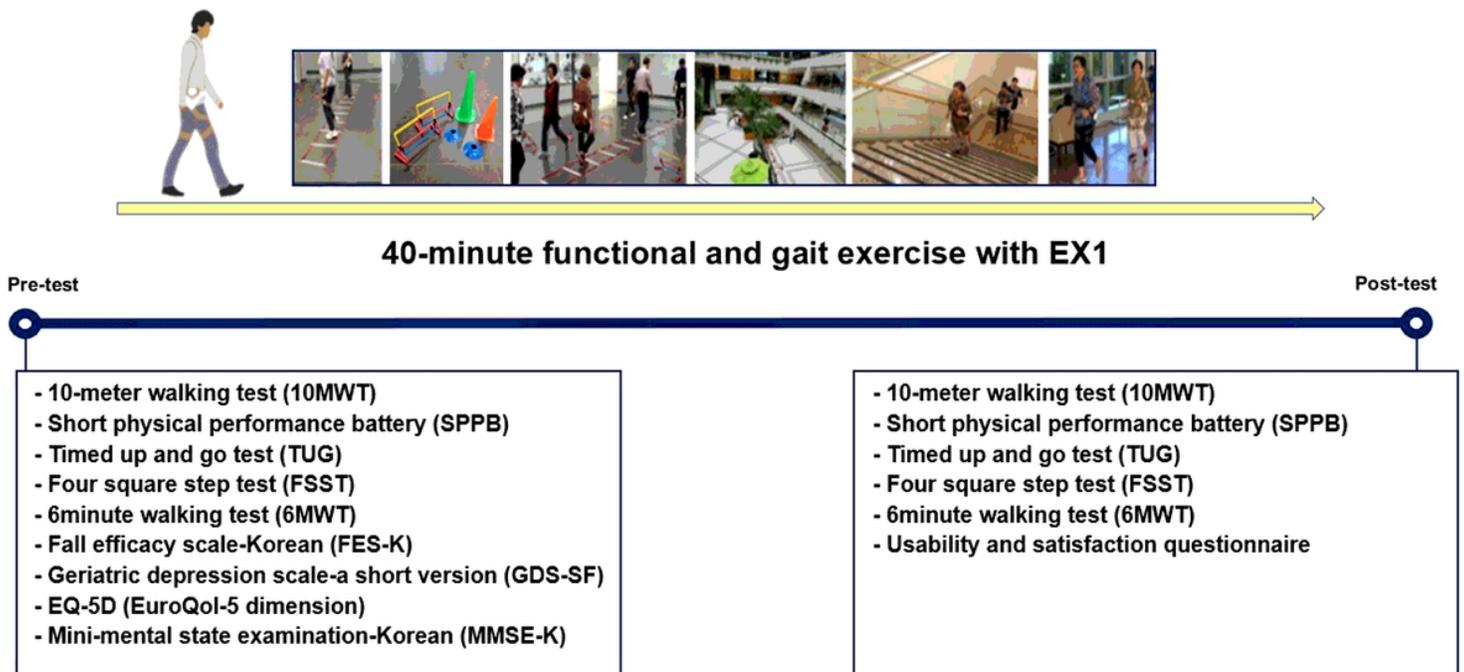


Figure 1

Experimental protocol



Figure 2

EX1 developed by Samsung Electronics

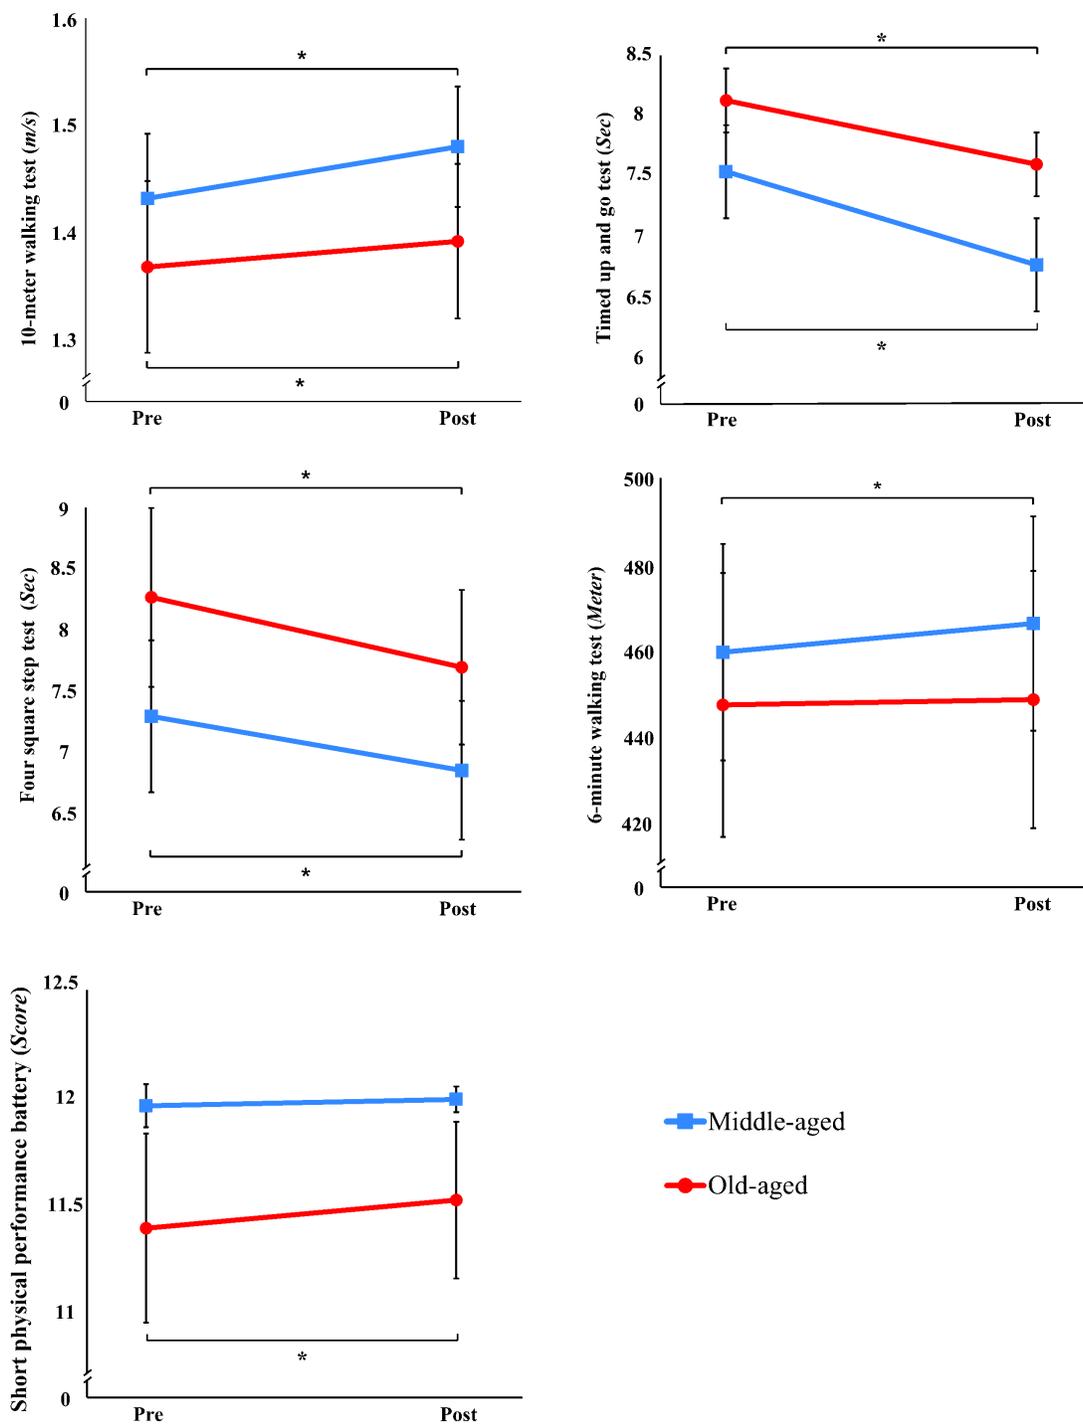


Figure 3

Changes in Physical function. **a)** 10-meter walking test; **b)** Timed Up and Go test; **c)** Four Square Step Test; **d)** 6 Minutes Walking Test; **e)** Short Physical Performance Battery ($*p < 0.05$).

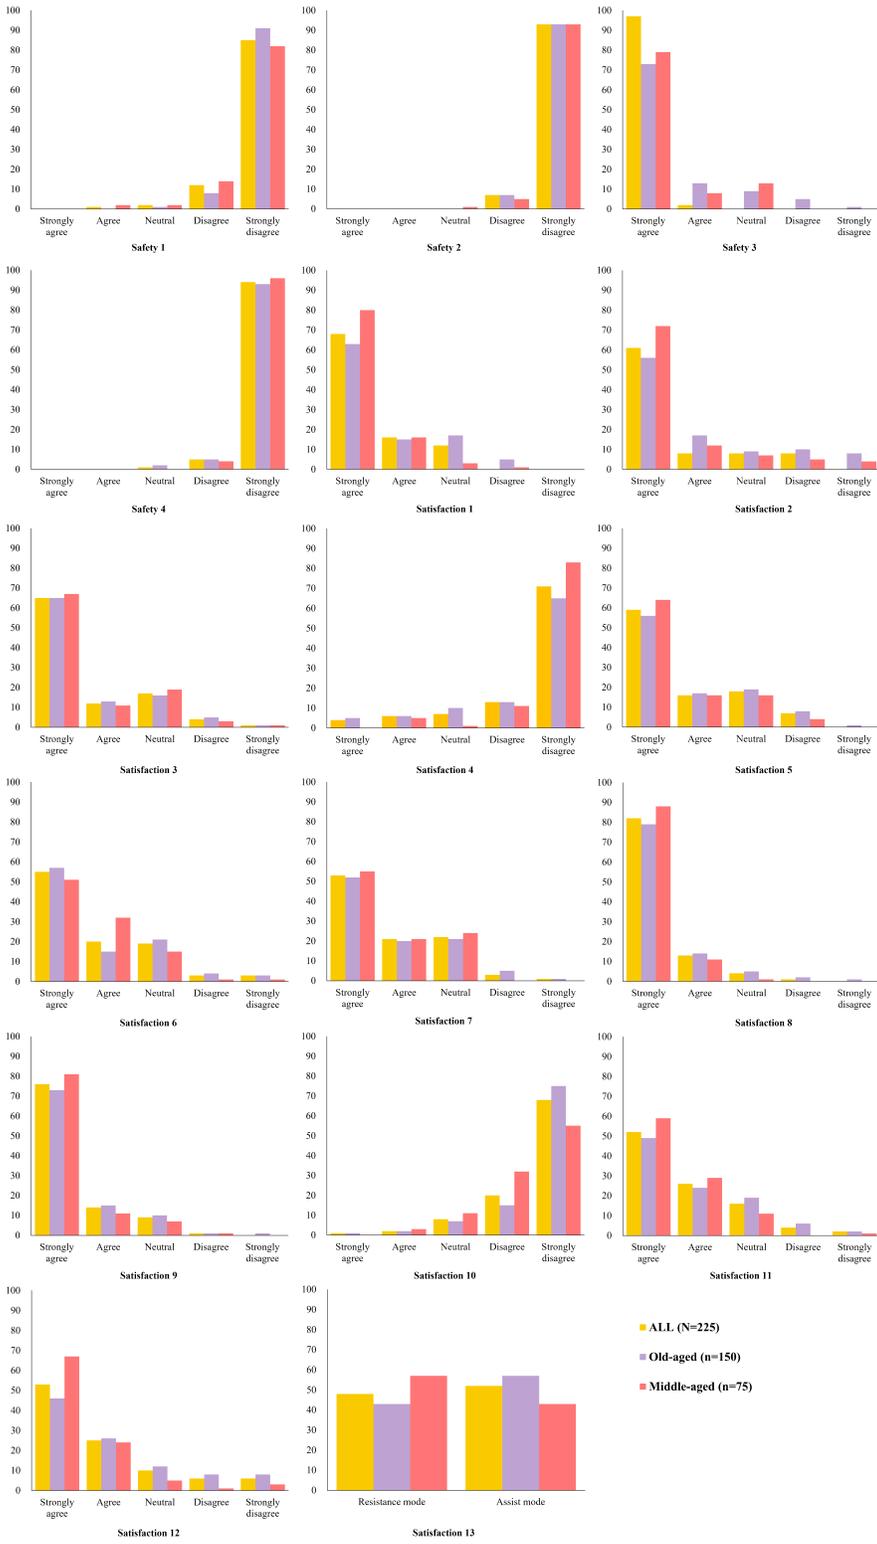


Figure 4

Responses to the questionnaire about usability and satisfaction of the EX1. The items of the usability and satisfaction evaluation include the safety of wearing, the risk of falling, the ease of operation, the feeling of weight, the fit, and the noise of the EX1. Refer to Table 3 for the usability and satisfaction questionnaire.

Supplementary Files

This is a list of supplementary files associated with this preprint. Click to download.

- [3.Supplementary.docx](#)