

Accuracy of pilot balloon palpation in small sized tubes compared to large sized tubes: A prospective observational study

MinGi Ban

Yonsei University College of Medicine, Yonjin Severance Hospital

So Yeon Kim

Yonsei University College of Medicine

Min Soo Kim

Yonsei University College of Medicine

Wyun Kon Park

Yonsei University College of Medicine

Sei Han Song

Yonsei University College of Medicine

Dongkwan Skin

Yonsei University College of Medicine

Hyun Joo Kim (✉ jjollong@gmail.com)

Yonsei University College of Medicine

Research Article

Keywords: cuff, endotracheal tube, intracuff pressure, palpation, pilot balloon

Posted Date: April 28th, 2022

DOI: <https://doi.org/10.21203/rs.3.rs-1595731/v1>

License:   This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

Abstract

Purpose

After inflating the cuff of the endotracheal tube, the pressure of the cuff should be evaluated as to whether it is appropriate for ventilation. The most commonly used method is pilot balloon palpation. This study evaluated whether the size of the tracheal tube influenced the accuracy of pilot balloon palpation.

Methods

A prospective observational analysis of 208 patients intubated with an endotracheal tube of internal diameter (ID) 6.0 or 8.0 was conducted. An anesthesiologist first judged whether the cuff pressure was appropriate by manual pilot balloon palpation, and then measured the cuff pressure with a pressure gauge. If the cuff pressure exceeded 20–30 cmH₂O, it was defined as a false recognition.

Results

The intracuff pressure was significantly higher in ID 6.0 tube than in the ID 8.0 tube (41.9 ± 18.8 cmH₂O vs. 30.3 ± 11.9 cmH₂O, $p < 0.001$). The number of patients that were mistakenly perceived to have appropriate cuff pressure by pilot balloon palpation was significantly higher in the ID 6.0 group compared to the ID 8.0 group (85 (81.7%) vs. 64 (61.5%), $p = 0.001$).

Conclusions

The incidence of inaccurate assessment of adequate cuff pressure when determining cuff pressure by pilot balloon palpation was higher in the relatively smaller endotracheal tube size group compared to the larger endotracheal tube size group. Therefore, use of a pressure gauge to confirm adequate pressure is recommended especially when using a smaller tube size.

1 Introduction

The endotracheal tube has a cuff which must be inflated to seal the trachea for appropriate mechanical ventilation. With an insufficiently inflated cuff, there is possibility of an oxygen leak that may lead to ineffective ventilation as well as an increase in the risk of pneumonia by allowing aspiration by secretions from the mouth. [1]. On the contrary, if the cuff is excessively inflated, the cuff strongly compresses the mucous membrane on the inner wall of the trachea, which may cause ischemia and complications such as sore throat, vocal cord paralysis, tracheal rupture, subglottic stenosis, and nerve damage after surgery [2, 3]. Therefore, it is recommended that the cuff should be inflated to an appropriate pressure to allow mechanical ventilation without causing complications.

When the cuff is inflated with air, the size of the cuff increases and the cuff contacts the tracheal wall, pushing against the tracheal mucosa [4]. It has been reported that the pressure impairing the perfusion of trachea and the pressure in the cuff are the same [5]. Accordingly, it is recommended that the cuff in properly inflated and determined within the range of 20–30 cmH₂O [1, 4]. Among the various methods of evaluating appropriate cuff pressure, the most commonly used method is the method of recognizing the pressure by tactile sensation by directly touching the pilot balloon between fingers, and it has been reported to be used in about 44–51% [6, 7]. The tactile perception method was reported to be more inaccurate than using a pressure gauge [8], but hospitals still do not use a pressure gauge in every operating room due to either cost reasons or inconvenience or both. [9]. In our hospital, because not all operating rooms are equipped with a pressure gauge, pilot balloon palpation is still most commonly applied. Therefore, if we can determine the risk factors of increasing inaccurate assessment, a focused strategy of using a pressure gauge can be established to ensure safe anesthesia for those patients who particularly need a pressure gauge assessment rather than tactile assessment.

Since the pilot balloon has smaller radius than the cuff, there is a risk that the wall tension perceived by the tactile sensation is different according to the Laplace's law, and the estimated pressure is lower than the actual pressure of the cuff [10]. Other studies have argued that if the size of the pilot balloon is made as large as the cuff, the probability of misrecognizing the actual pressure of the cuff will decrease [11, 12]. Nevertheless, although the risk factors of cuff over-inflation or under-inflation are analyzed, studies on risk factors that make cuff pressure misrecognized have not been conducted in clinical practice. Therefore, we decided to evaluate the effect of different sizes of endotracheal tubes on the degree of cuff swelling and the accuracy of the tactile perception method.

This study hypothesized that the incidence of false recognition was higher in internal diameter (ID) 6.0 tubes than in ID 8.0 tubes when the cuff pressure was estimated by palpating the pilot balloon after endotracheal intubation. The primary outcome is the rate of incidence that was erroneously recognized when pressure was estimated by palpating the pilot balloon.

2 Methods

This prospective, single-center, observational study was approved by the institutional review board of Severance Hospital, Yonsei University Health System (Seoul, Republic of Korea; numbers: 4-2019-0104; April 1, 2019). The study protocol was registered at www.clinicaltrials.gov (NCT03938506, May 9, 2019). Written informed consent was obtained from all patients participating in this study. From January 2020 to November 2020, we enrolled male patients aged 20 years or older scheduled to undergo surgery under general anesthesia using an endotracheal tube of size ID 6.0 or 8.0. Exclusion criteria included the following: patients with a tracheostomy tube; and patients with abnormal tracheal findings such as an endotracheal mass, tracheal deviation, and/or tracheal narrowing.

Standard monitors for pulse oximetry, 3-lead electrocardiography, and non-invasive blood pressure measurement were attached. Anesthesia was induced using 1–2 mg kg⁻¹ propofol (Fresofol 1% MCT;

Fresenius Kabi Austria GmbH, Graz, Austria), 0.5–1.0 µg kg⁻¹ remifentanyl (Ultian; Hanlim Pharm. Co., Ltd., Seoul, Korea), and 0.6–1.0 mg kg⁻¹ rocuronium (Rocumeron; Ilsung Pharmaceuticals Co., Ltd., Seoul, Korea). Mask ventilation was performed using oxygen at 5 L min⁻¹ and sevoflurane 4.0 vol %. After establishing a complete neuromuscular block, intubation was performed using videolaryngoscope with endotracheal tube of size ID 6.0 or 8.0 (Shiley™ Ta-perGuard oral tracheal tube, Covidien, MA, USA). The cuff of tube was inflated by inserting air into the pilot balloon of tube. The anesthesiologists assessed the adequacy of degree of cuff inflation by palpating pilot balloon with their fingers. Breathing circuit was connected to the tube and mechanical ventilation was started using volume-controlled mode. Target tidal volume was 8 ml kg⁻¹ with a fresh gas flow of 2 L min⁻¹, respiratory rate of 12 breaths min⁻¹, inspiratory-expiratory ratio of 1:2, and positive end-expiratory pressure of 5 cmH₂O. After 30 seconds, intracuff pressure was measured using cuff manometer (Cuff Inflator/Pressure Gauge, Smiths Medical Inc, Kent, UK) and recorded. The intracuff pressure was considered inadequate if the pressure was out of the range of 20–30 cmH₂O [1, 4]. Then, the intracuff pressure was adjusted to 25 cmH₂O and surgery was proceeded. Patient characteristics such as age, height, weight, American Society of Anesthesiologists physical class, and endotracheal tube size were recorded.

The primary outcome was the incidence rate when the intracuff pressure of the endotracheal tube is not within the appropriate range of 20–30 cmH₂O. To determine sample size, we estimated the incidence of inadequate intracuff pressure based on previous report [9]. Based on the PASS (version 12, NCSS, LLC, Kaysville, Utah, USA), the required sample size was calculated to be 186 (assuming significant difference of incidence = 10%, Type I error = 5%, and power = 80%). In total, 208 participants were needed after accounting for a 10% dropout rate.

The intracuff pressure of endotracheal tube size ID 6.0 and 8.0 was compared using the Student's t-test. The number of patients who had adequate or inadequate intracuff pressure was compared between the endotracheal tube size ID 6.0 and 8.0 using Chi-square tests or Fisher's exact test. Clinically significant factors among the pre-operative characteristics, including age, height, weight, and tube size were entered into a multivariable logistic regression model to assess their impact on the incidence of in-adequate intracuff pressure. Values are presented as mean (SD) or numbers (percentages). Analyses were conducted using SAS software version 9.4 (SAS Institute Inc., Cary, NC). A P-value of < 0.05 was considered statistically significant.

3 Results

Of the 211 patients screened, 210 patients were eventually enrolled. Among them, 2 patients were dropped out due to request the surgeon for use of a different sized tube prior to surgery. Overall, 208 patients completed the study (Fig. 1) and no missing data were recorded for any patient. Patient baseline characteristics are summarized in Table 1.

Table 1
Patient demographics

N = 208		ID 6.0 tube (n = 104)	ID 8.0 tube (n = 104)	P-value
Age (year)		50.5 ± 16.6	45.2 ± 14.8	0.015
Height (cm)		170.7 ± 7.1	172.6 ± 6.7	0.054
Weight (kg)		71.6 ± 12.8	74.5 ± 11.2	0.090
American Society of Anesthesiologists class	1	42(40.1%)	49(47.1%)	0.264
	2	38(36.5%)	40(38.5%)	
	3	24(23.1%)	15(14.4%)	
Values are presented as mean ± SD or number (proportion). ID, internal diameter.				

The intracuff pressure was significantly higher in ID 6.0 tube than in the ID 8.0 tube (P < 0.001) (Table 2).

Table 2
Adequacy of intracuff pressure between ID 6.0 and ID 8.0 endotracheal tube.

	ID 6.0 tube (n = 104)	ID 8.0 tube (n = 104)	P-value
Intracuff pressure (cmH ₂ O)	41.9 ± 18.8	30.3 ± 11.9	< 0.001
Adequate intracuff pressure (cmH ₂ O)	25.7 ± 1.9	24.5 ± 3.2	0.068
Inadequate intracuff pressure (cmH ₂ O)	45.5 ± 18.9	34.0 ± 13.7	< 0.001
Intracuff pressure lower than 20cmH ₂ O (cmH ₂ O)	14.3 ± 3.0	14.8 ± 3.7	0.730
Intracuff pressure higher than 30cmH ₂ O (cmH ₂ O)	51.2 ± 14.5	40.4 ± 8.9	< 0.001
Patients, n (%)			0.001
With adequate intracuff pressure	19(18.3)	40(38.5)	
With inadequate intracuff pressure	85(81.7)	64(61.5)	
Patients, n (%)			
With inadequate pressure lower than 20cmH ₂ O	13(12.5)	16(15.4)	0.548
With inadequate pressure higher than 30cmH ₂ O	72(69.2)	48(46.2)	< 0.001
Values are presented as mean ± SD or number (proportion). ID, internal diameter.			

The number of patients who had inadequate intracuff pressure was significantly higher in ID 6.0 tube than in the ID 8.0 tube ($P < 0.001$). In univariable analysis, endotracheal tube size was significantly associated with inadequate cuff pressure. (Table 3) For multivariable analysis, endotracheal size was identified as a significantly independent risk factor for inadequate cuff pressure (odds ratio [OR] 0.36; 95% CI, 0.18–0.68; $p = 0.002$). (Table 3)

Table 3
Univariate and multivariate analysis inadequate intracuff pressure

	Univariate analysis	P-value	Multivariate analysis	P-value
	OR (95% CI)		OR (95% CI)	
Tube size	0.36(0.19–0.68)	0.002	0.36(0.18–0.68)	0.002
ID 6.0 / ID 8.0				
Age	1.01(0.99–1.03)	0.568	1.01(0.98–1.03)	0.687
Height	1.01(0.96–1.05)	0.810	1.05(0.99–1.11)	0.135
Weight	0.99(0.96–1.01)	0.236	0.98(0.95–1.01)	0.123
OR, odds ratio; CI, confidence interval; ID, internal diameter.				

4 Discussion

In this study, we compared the adequacy of estimating intracuff pressure by palpating the pilot balloon in different sized endotracheal tubes. Our results showed that an endotracheal tube with a smaller inner diameter was more likely to be assessed with an inadequate cuff pressure compared to a larger endotracheal tube when manually palpated.

In our study, when estimating the intracuff pressure by palpating the pilot balloon, nearly 72% of our patients overall were found to be inadequately assessed as appropriate. As our hospital teaches the importance of appropriately adjusting the cuff pressure, and anesthesiologists who have experience controlling cuff pressure using a manometer participated in our study, we expected there would be more cases of accurate judgement. Compared to previous studies where there were incidences up to 90% of misperception when surveyed in various environments such as the operating room and intensive care unit [8, 9, 13], it could be perceived that there were similar or fewer cases of misinterpretation in our hospital. Nevertheless, the inadequate rate reached over 70%, and the method of palpating the pilot balloon shows low reliability. If the application of a pressure gauge in all patients is difficult for reasons for cost and inconvenience, the probability of accurately estimating cuff pressure could be improved by having training courses [8, 9]. Education about cuff pressure is recommended and a focused protocol should be instated so that specific patient groups with high risk profiles are targeted for standardized use of a pressure gauge.

Risk factors causing inappropriate intracuff pressure estimation were investigated, and only tube size among the age, height and weight were determined to be a risk factor. In previous studies, the risk factors of cuff over-inflation and under-inflation were reported as hypothermia, duration of intubation, absence of sedation, and changes in head and neck position [14–16]; however, there have not been any studies to analyze whether the size of the tube is a risk factor of the misperception. In this study, we found for the first time that as the inner diameter of the tube is smaller and the difference between the patient's airway diameter and tube size increases, it is possible to seriously error in manually estimating the intracuff pressure by the pilot balloon. A probable cause to why the smaller tube is more inaccurate may be because the tube with the smaller inner diameter also has a smaller outer diameter. Thus, when the cuff is inflated, a larger amount of air is required to inflate the cuff to reach the tracheal wall. In addition, the taperguard tube has a conical cuff shape with a narrower distal part of the cuff, and this allows for a more limited part of the outer surfaces of the cuff to contact the inner wall of the trachea when being sealed. When the cuff is inflated, the smallest tube will touch the tracheal wall at its largest circumference, and the larger tube will reach the tracheal wall even if the cuff is inflated slightly, and longitudinal folds are likely to occur with the wide contact of the outer surfaces of the cuff [17]. We think that the area of the outer surface of the cuff in contact with the tracheal inner wall and whether the cuff has more remaining extra volume for inflation might be one of the causes of our findings. Looking more closely at the cases where the cuff pressure was inappropriate, for ID 6.0 tube, the mean pressure was 45.5 ± 18.9 cmH₂O, and for ID 8.0 tube, the mean pressure was mistaken to 34.0 ± 13.7 cmH₂O. Inadequate measurements of more than 30 cmH₂O occurred in 69.2% for ID 6.0 tubes and 46.2% for ID 8.0 tubes. In comparison, cases of inadequate measurements of less than 20 cmH₂O was lower at 12.5% for ID 6.0 tubes and 15.4% for ID 8.0 tubes. This means that when we manually assessed the ID 6.0 tube pilot balloon, there was a tendency to feel more 'flabby' or less inflated than the ID 8.0 tube pilot balloon, so by adding a larger amount of air, the cuff pressure measured higher than the recommended range [18]. This is probably because the ID 6.0 tube needs a larger amount of air to contact the tracheal wall, and the difference in volume between the pilot balloon and the cuff increased, and the wall tension was felt incorrectly according to the Laplace's law [10]. In addition, in clinical practical, because the tube size ID 7.0–8.0 are more generally used when performing general anesthesia, it may be presumed that there is a familiarity with these two tube sizes compared to smaller sizes due to years of training. Therefore, the use of a pressure gauge should always be considered when using a size or type of tubes that are used only intermittently for specific surgeries rather than size or type of tubes that are more commonly used in each hospital.

There are several limitations in this study. First, we only investigated male patients. The reason for this was to examine different sized tubes under similar trachea size because the size of trachea differs according to sex [19]. We believe that the same principles will apply in women. Second, the results may vary depending on the type of tracheal tube. Each tracheal tube has a different outer diameter even with the same inner diameter, and the shape and material of the cuff and pilot balloon are different [5, 12]. In this study, we evaluated the cuff with the high volume low pressure, tapered shape with polyvinylchloride

material which was used in our institution. Therefore, further research on various tubes is needed in the future.

5 Conclusion

In conclusion, when estimating and adjusting the cuff pressure by touching the pilot balloon, the smaller size endotracheal tube has a higher risk of incorrectly assessing the pressure compared to the larger size tube. In particular, it is possible to erroneously judge that the pressure is low and inflate excessively, which could result in a very high pressure outside the recommended range. Therefore, when using a smaller tube, a pressure gauge should be considered for accurate measurement of cuff pressure in safe practice.

Declarations

Funding The authors declare that no funds, grants, or other support were received during the preparation of this manuscript.

Competing Interests The authors have no relevant financial or non-financial interests to disclose.

Author Contributions All authors contributed to the study conception and design. Material preparation, data collection and analysis were performed by MinGi Ban, So Yeon Kim and Hyun Joo Kim. The first draft of the manuscript was written by MinGi Ban and all authors commented on previous versions of the manuscript. All authors read and approved the final manuscript

Ethics Approval The study was conducted in accordance with the Declaration of Helsinki, and approved by the Institutional Review Board of Severance Hospital, Yonsei University Health System (Seoul, Republic of Korea; numbers: 4-2019-0104; April 1, 2019). The study protocol was registered at www.clinicaltrials.gov (NCT03938506, May 9, 2019).

Consent to participate Informed consent was obtained from all subjects involved in the study. Written informed consent has been obtained from the patients to publish this paper.

References

1. Bouadma L, Wolff M, Lucet JC. Ventilator-associated pneumonia and its prevention. *Curr Opin Infect Dis.* 2012;25(4):395–404.
2. Sultan P, Carvalho B, Rose BO, Cregg R. Endotracheal tube cuff pressure monitoring: a review of the evidence. *J Perioperative Pract.* 2011;21(11):379–86.
3. Liu J, Zhang X, Gong W, Li S, Wang F, Fu S, et al. Correlations between controlled endotracheal tube cuff pressure and postprocedural complications: a multicenter study. *Anesth Analg.* 2010;111(5):1133–7.
4. Seegobin RD, van Hasselt GL. Endotracheal cuff pressure and tracheal mucosal blood flow: endoscopic study of effects of four large volume cuffs. *Br Med J (Clin Res Ed).*

- 1984;288(6422):965–8.
5. Chenelle CT, Itagaki T, Fisher DF, Berra L, Kacmarek RM. Performance of the PneuX System: A Bench Study Comparison With 4 Other Endotracheal Tube Cuffs. *Respir Care*. 2017;62(1):102–12.
 6. Lee J, Reynolds H, Pelecanos AM, van Zundert AA. Bi-national survey of intraoperative cuff pressure monitoring of endotracheal tubes and supraglottic airway devices in operating theatres. *Anaesth Intensive Care*. 2019;47(4):378–84.
 7. Miao I, Jee R, Pysyk CL. Under pressure: an audit of airway device pressures. *Can J Anaesth*. 2018;65(6):726–7.
 8. Giusti GD, Rogari C, Gili A, Nisi F. Cuff pressure monitoring by manual palpation in intubated patients: How accurate is it? A manikin simulation study. *Aust Crit Care*. 2017;30(4):234–8.
 9. Ozcan ATD, Doger C, But A, Kutlu I, Aksoy SM. Comparison of endotracheal tube cuff pressure values before and after training seminar. *J Clin Monit Comput*. 2018;32(3):527–31.
 10. Pisano A. Pitfalls From Physics: Why We Can't "Feel" the Tube Cuff Pressure With Our Fingers. *Anesth Analg*. 2017;124(4):1368.
 11. Pisano A, Verniero L, Galdieri N, Corcione A. Assessing the correct inflation of the endotracheal tube cuff: a larger pilot balloon increases the sensitivity of the 'finger-pressure' technique, but it remains poorly reliable in clinical practice. *J Clin Monit Comput*. 2018.
 12. Janossy KM, Pullen J, Young D, Bell G. The effect of pilot balloon design on estimation of safe tracheal tube cuff pressure. *Anaesthesia*. 2010;65(8):785–91.
 13. Mendelsohn AH, Mukdad L, Dhillon A. High intraoperative endotracheal tube cuff pressure incidence and clinical impact. *Can J Anaesth*. 2018;65(3):331–2.
 14. Kako H, Alkhatib O, Krishna SG, Khan S, Naguib A, Tobias JD. Changes in intracuff pressure of a cuffed endotracheal tube during surgery for congenital heart disease using cardiopulmonary bypass. *Paediatr Anaesth*. 2015;25(7):705–10.
 15. Kako H, Krishna SG, Ramesh AS, Merz MN, Elmaraghy C, Grischkan J, et al. The relationship between head and neck position and endotracheal tube intracuff pressure in the pediatric population. *Paediatr Anaesth*. 2014;24(3):316–21.
 16. Nseir S, Brisson H, Marquette CH, Chaud P, Di Pompeo C, Diarra M, et al. Variations in endotracheal cuff pressure in intubated critically ill patients: prevalence and risk factors. *Eur J Anaesthesiol*. 2009;26(3):229–34.
 17. Deem S, Treggiari MM. New endotracheal tubes designed to prevent ventilator-associated pneumonia: do they make a difference? *Respir Care*. 2010;55(8):1046–55.
 18. Hoffman RJ, Dahlen JR, Lipovic D, Stürmann KM. Linear correlation of endotracheal tube cuff pressure and volume. *West J Emerg Med*. 2009;10(3):137–9.
 19. Karmakar A, Pate MB, Solowski NL, Postma GN, Weinberger PM. Tracheal size variability is associated with sex: implications for endotracheal tube selection. *Ann Otol Rhinol Laryngol*. 2015;124(2):132–6.

Figures

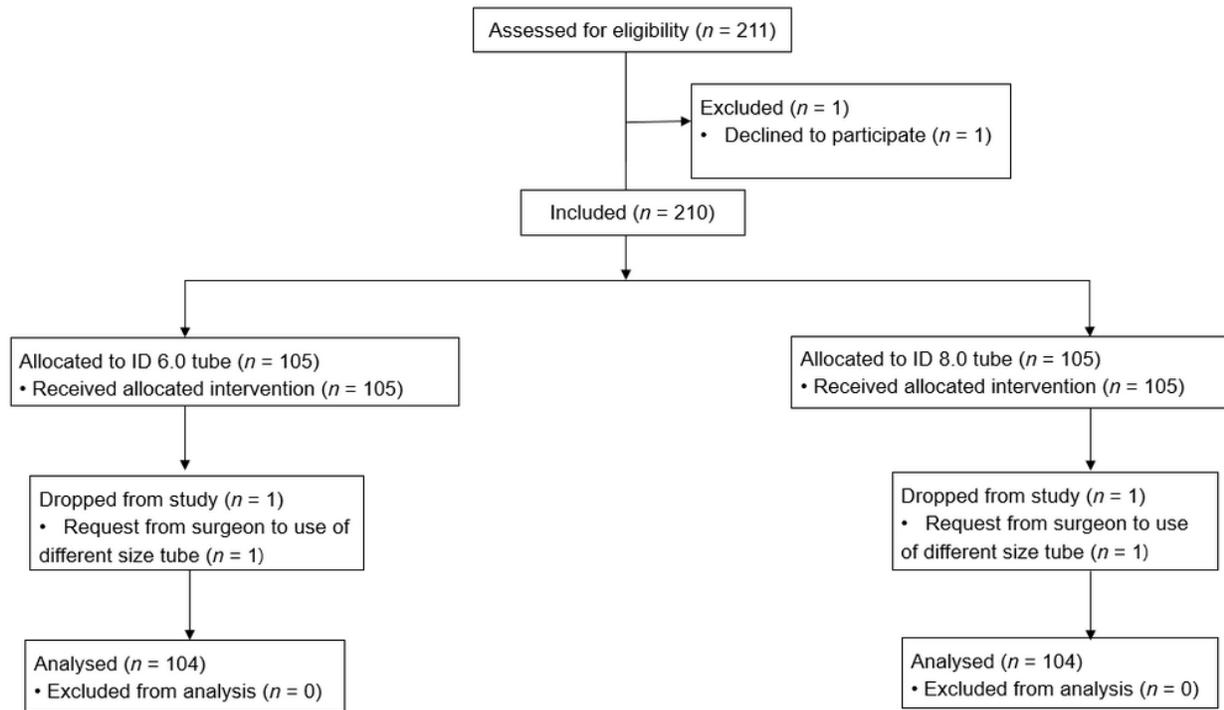


Figure 1

Demographics