

# Naturalistic visualization of reaching movements using head-mounted displays improves movement quality and proves high usability compared to conventional computer screens

**Nicolas Wenk**

University of Bern

**Karin A. Buetler**

University of Bern

**Joaquin Penalver-Andres**

University of Bern

**René M. Müri**

University of Bern

**Laura Marchal-Crespo** (✉ [laura.marchal@unibe.ch](mailto:laura.marchal@unibe.ch))

University of Bern

---

## Research Article

**Keywords:** Virtual reality, Augmented reality, Head-mounted display, Neurorehabilitation, Movement quality, Cognitive load, Motivation, Usability, Stroke

**Posted Date:** June 22nd, 2022

**DOI:** <https://doi.org/10.21203/rs.3.rs-1749644/v1>

**License:**  This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

---

## RESEARCH

# Naturalistic visualization of reaching movements using head-mounted displays improves movement quality and proves high usability compared to conventional computer screens

Nicolas Wenk<sup>1</sup>, Karin A. Buetler<sup>1</sup>, Joaquin Penalver-Andres<sup>1</sup>, René M. Müri<sup>2,3</sup> and Laura Marchal-Crespo<sup>1,4\*</sup>

## Abstract

**Background:** The relearning of movements after brain injury can be optimized by providing intensive, meaningful, and motivating training using virtual reality (VR). However, most current solutions use two-dimensional (2D) screens, where patients interact via symbolic representations of their limbs (e.g., a cursor). These 2D screens lack depth cues, potentially deteriorating movement quality and increasing cognitive load. Head-mounted displays (HMDs) have great potential to provide naturalistic movement visualization by incorporating improved depth cues, reduce visuospatial transformations by rendering movements in the space where they are performed, and preserve eye-hand coordination by showing an avatar – with immersive VR (IVR) – or the user’s real body – with augmented reality (AR). However, elderly populations might not find these novel technologies usable, hampering potential motor and cognitive benefits.

**Methods:** We compared movement quality, cognitive load, motivation and system usability in twenty elderly participants (>59 y.o.) while performing a dual motor-cognitive task with different visualization technologies: IVR HMD, AR HMD, and a 2D screen. We evaluated participants’ self-reported cognitive load, motivation, and usability using questionnaires. We also conducted a pilot study with five brain-injured patients comparing the visualization technologies while using an assistive device.

**Results:** Elderly participants performed straighter, shorter duration, and smoother movements when the task was visualized with the HMDs than screen. The IVR HMD led to shorter duration movements than AR, and both HMDs were associated with shorter movement duration than the screen. Movement onsets were shorter with IVR than AR, and shorter for both HMDs than the screen, potentially indicating facilitated reaction times due to reduced cognitive load. No differences were found in the questionnaires regarding cognitive load, motivation, or usability between technologies in elderly participants. Both HMDs proved high usability in our small sample of patients.

**Conclusions:** HMDs are a promising technology to be incorporated into neurorehabilitation, as their more naturalistic movement visualization improves movement quality compared to conventional screens. HMDs demonstrate high usability, without decreasing participants’ motivation, and might potentially lower cognitive load. Our preliminary clinical results suggest that brain-injured patients may especially benefit from more immersive technologies. However, larger patient samples are needed to draw stronger conclusions.

**Keywords:** Virtual reality; Augmented reality; Head-mounted display; Neurorehabilitation; Movement quality; Cognitive load; Motivation; Usability; Stroke

\*Correspondence: [laura.marchal@unibe.ch](mailto:laura.marchal@unibe.ch)

<sup>1</sup>Motor Learning and Neurorehabilitation Laboratory, ARTORG Center for Biomedical Engineering Research, University of Bern, Bern, Switzerland

Full list of author information is available at the end of the article

## Introduction

Stroke is one of the most important sources of permanent disability worldwide with over 12 million new cases every year worldwide [1]. Stroke is defined as

a “*disturbance of cerebral function, lasting more than 24 hours or leading to death, with no apparent cause other than of vascular origin*” [2]. Similar to other neurological dysfunctions – e.g., Parkinson’s disease, traumatic brain injury –, stroke survivors usually suffer from motor impairments such as muscle weakness, reduced movement workspace, and loss of movement quality, which limit their ability to perform activities of daily living (ADL) independently. Importantly, 21-44 % of stroke survivors also suffer from cognitive impairments that impact among others, memory, language, orientation, attention, and/or executive function [3].

When the potential for recovery remains – e.g., when there is no substantial damage to the corticospinal tract [4, 5] – relearning of movements after a brain injury can be achieved by enrolling into neurorehabilitation interventions. Neurorehabilitation aims to enhance patients’ functional movements during ADLs [6] and is accepted to be a form of motor (re)learning [7]. Neurorehabilitation can be optimized by promoting intensive [8] and task-specific [9] movement training that provides functional multi-sensory input to the central nervous system [10], known to lead to synaptic plasticity in the brain [11].

Robotic devices, together with virtual reality (VR) games, can provide intensive training in a motivating virtual environment (VE). VR allows patients to visualize their movements in a VE and can provide meaningful goal/task-oriented exercises – e.g., realistic simulations of the ADLs to retrain – that can be adapted to the patients’ specific needs. Importantly, the use of VR has been shown to increase patients’ motivation – a factor known to enhance functional recovery [12, 13, 14] and facilitate motor learning through the release of dopamine known to support memory consolidation and neuroplasticity [15]. A recent meta-analysis of randomized clinical trials concluded that VR is, indeed, a promising technology for upper limb motor rehabilitation in post-stroke patients [16].

However, during conventional robotic VR-based neurorehabilitation, the VE is usually displayed on a two-dimensional (2D) surface (e.g., 2D screen) and patients interact with the VE via a symbolic virtual representation of their limbs (e.g., a cursor). Although this provides useful visual feedback, 2D screens draw patients’ attention away from their limbs, breaking the eye-hand coordination. This eye-hand coordination is known to aid goal-oriented movements, which might be already affected in brain-injured patients [17]. Furthermore, the reduced depth cues in 2D screens that do not provide stereo vision and the visuospatial transformation between the visualized movements space and the physical movement space might add an extra cognitive load to the patients [18, 19]. This could lead to

a two-step learning phase, where patients first learn the visuospatial transformation before being able to focus on learning the physiological movements, wasting valuable rehabilitation time, as observed during robotic training with 2D screens [20]. Finally, most of the tasks used to evaluate the benefit of VR training on motor learning and transfer are rather simple to be easily controlled (e.g., reaching on a plane), yet those deviate from the movements usually performed in ADLs (e.g., reaching in the 3D space) [6].

Low-cost off-the-shelf Head-Mounted Displays (HMD) are now widely available, offering the possibility to provide a realistic virtual representation of the patient’s own limbs (avatar) in immersive VR (IVR) or the possibility of projecting virtual elements while still visualizing the patient’s own limbs with augmented reality (AR). The use of different VR displays might result in different motor performance compared to real movements [21]. For example, reaching movements performed towards targets located in the vertical plane have been shown to be slower, shorter, less straight, and less accurate when visualized on a 2D screen than movements performed in real life [19], while when using HMDs, movements seemed closer to the ones performed towards targets in the real life [22]. In a previous experiment with healthy young participants, we found that IVR HMD is associated with better movement quality in a 3D reaching task than 2D screens, especially when moving across several dimensions (horizontal, vertical, and in depth) [23]. Different visualization technologies could also have a different effect on participants’ cognitive load and psychological affects, e.g., motivation and usability. Indeed, in our previous experiment, we observed that healthy young participants’ motivation and system usability were higher with the IVR HMD compared to the 2D screen [24]. However, the visualization technology did not significantly impact their cognitive load, neither when measured with a parallel cognitive task [23], nor with subjective reports [24].

Thus, IVR and AR HMDs might offer benefits over 2D screens. First, their improved depth cues (over 2D screens) allow higher **movement quality** [25, 23]. Second, by displaying the movement in the same space where it is performed, the visuospatial transformation is reduced, potentially lowering the patients’ **cognitive load** [18]. Third, by using an animated avatar, the eye-hand coordination [17] could be preserved [18]. This more naturalistic interaction could potentially improve the system **usability**, ultimately increasing the inclusion and adherence of patients into VR-based interventions [24]. The patient’s **motivation** might also increase, either directly due to this more naturalistic interaction, or indirectly due to an increased

perceived competence elicited by the improved movement quality. However, although HMDs are slowly entering the rehabilitation context, there is currently little understanding of their impact on neurorehabilitation [26, 27, 16].

Brain injuries are more preeminent at older ages. Furthermore, cognitive decline is associated with participants' old age that might limit the usability of 2D screens in motor training [28, 29]. Therefore, in this study, we aimed at reproducing our previous study [23, 24] with two different populations, namely, with 20 healthy elderly participants (>59 y.o.; **Experiment 1**) and a small group of five acute brain-injured patients (**Experiment 2**). To facilitate the experiment with brain-injured patients, who suffered from motor impairments, we interfaced our VR/AR setup with a weight-support rehabilitation device (Arneo® Spring, Hocoma, Switzerland).

Based on previous results obtained in healthy young participants [23, 24, 18, 25], we formulated the following hypotheses: (1) IVR HMD would elicit better movement quality, less cognitive load, higher motivation, and a higher usability compared to the 2D screen; (2) With the 2D screen, we also expected that the movement quality would worsen when the reaching movement requires moving in the depth dimension at the same time than in another dimension (vertical and/or horizontal) compared to movements that do not require using the depth direction. We expected to see differences between visualization technologies in the cognitive load of elderly participants and brain-injured patients, as they are less cognitively fit than the healthy young participants from our previous experiment. Since we did not find conclusive results for the AR HMD in our previous study in terms of movement quality, cognitive load, motivation, and usability, we did not formulate hypotheses for this specific visualization technology, but kept it in the protocol to gather insights about the use of AR within aging and brain-injured populations.

## Methods

### Experiment 1 - Healthy Elderly Participants

#### Participants

Twenty participants without known motor or cognitive disorders aged from 60 to 89 years ( $74.22 \pm 8.11$ ) and without severe visual impairment provided written informed consent to participate in this first experiment. Fourteen participants were strongly right-handed, one was mixed right-handed, and one was mixed left-handed [30], based on the "Edinburgh Handedness Inventory" [31]. Other demographic data is available in Table 1. Participants were recruited via word-of-mouth. The study was approved by the local Ethics

Committee (ref.: 2017-02,195) and conducted in compliance with the Declaration of Helsinki. Participants did not receive any compensation for their participation in the study.

#### Experimental Setup

The experiment was performed in a room with only artificial and controllable lighting (Fig. 1 a). The participants sat on a lockable-wheeled chair set at a pre-defined fixed location in the room.

The IVR HMD used in the experimental setup (Fig. 1 a) was an HTC Vive Pro (HTC, Taiwan & Valve, USA), tracked with two SteamVR™ Base Station 2.0. Participants wore three *HTC Vive trackers (2018)* attached to their right arms and shoulders, while holding an *HTC Vive controller (2018)* in their right hand (HTC, Taiwan & Valve, USA). We calibrated the IVR HMD by measuring the participants' interpupillary distance and setting it with the dedicated wheel.

The AR HMD used was a Meta 2 (Meta Company, USA), with its "simultaneous localization and mapping" (SLAM) function disabled. The head tracking for AR was performed using an *HTC Vive tracker (2018)* fixated on the HMD to prevent that differences in tracking performance would affect our experiment results. To calibrate the AR HMD, participants were guided by the experimenter through the Meta 2 eye calibration software ( $\sim 5$  min).

The 2D computer screen used was a Samsung S24E560 (Samsung, South Korea) with a diagonal of 24 inches and located on a table at an approximate distance of 1 m from the participant's body. To align the tracking reference system to the participants for the 2D screen modality, we needed to know the participant's initial head position and orientation. Therefore, participants wore the Meta 2 HMD tracked with the *HTC Vive tracker (2018)* in a first initialization phase. The experimenter quickly removed the HMD after calibration.

We employed a computer to run the VE and the experimental protocol with Windows 10 Home 64 bit edition (Microsoft, USA), 32 GB of DDR3 working memory, Intel Core i7-8700K (Intel Corporation, USA), and an NVIDIA GeForce GTX 1080 Ti (NVIDIA Corporation, USA).

#### Reaching and Cognitive Tasks

Participants were requested to perform a motor reaching task and, in parallel, a cognitive counting task. In the motor task, participants had to reach for and touch fruits (oranges, apples, and pears) that appeared at 22 pre-randomized locations within a pre-defined workspace of dimensions 35.88 x 28.47 x 37.26 cm (width x height x depth). The workspace was defined

**Table 1** Elderly participants' demographic data. Experience with VR and video gaming rated from 1 ("Not at all") to 7 ("Very much")

#	Gender	Age	Highest educational achievement	Experience with VR	Experience with video games	Hours spent playing video games per week in the last month
1	Male	84	Apprenticeship	1	2	3
2	Female	82	Apprenticeship	1	1	0
3	Female	68	High school	1	1	0
4	Female	72	Apprenticeship	1	1	0
5	Male	64	University or equivalent	2	1	0
6	Female	64	University or equivalent	1	1	0
7	Female	70	Apprenticeship	1	1	0
8	Male	60	University or equivalent	1	2	0
9	Male	67	Apprenticeship	1	1	0
10	Male	64	High school	1	2	3
11	Female	89	Apprenticeship	1	1	0
12	Female	71	Apprenticeship	4	1	0
13	Male	85	Apprenticeship	1	1	0
14	Male	84	University or equivalent	2	2	0
15	Male	76	High school	5	5	0
16	Female	78	University or equivalent	1	1	0
17	Male	73	University or equivalent	2	3	0
18	Male	77	University or equivalent	1	1	0
19	Male	72	Apprenticeship	5	5	0.5
20	Male	75	Apprenticeship	4	6	2

along three perpendicular axes: horizontal, vertical, and depth. The horizontal and vertical axes matched the horizontal and vertical screen coordinates, which rendered the VE from the avatar's head location when looking at the center of the screen (origin of the VE Cartesian coordinate system). The workspace center was located at 19.8 cm on the right and at 44.4 cm in front of the transverse plane and 19.98 cm under the participants' eyes on the longitudinal axis.


Two potential fruit locations within the workspace used only the depth axis (one on each side of the workspace center; Fig. 1 c, locations in yellow). Eight potential locations did not use the depth at all (two using only the horizontal axis, two using only the vertical one, and four combining the horizontal and vertical axes; Fig. 1, c, locations in red). Finally, twelve potential locations included the depth axis combined with at least another one (eight used combinations of the three axes and four combined the depth with the horizontal axis; Fig. 1, c, locations in orange).

Only one fruit was visible at a time. To touch a fruit, participants had to reach towards it and "touch" it with a virtual blue sphere attached to the controller. As soon as the fruit was "touched", it disappeared and a green sphere appeared in the center of the workspace. Participants were asked to then touch the green sphere (with the blue one) and to remain in contact with it until it disappeared and the next fruit appeared (unless the trial was over). The participants had to touch a total of 102 fruits, moving from the initial position marked by the green sphere, which were grouped into eight blocks of 6, 12, 12, 12, 18, 18, 18, and 6 fruits each. The green sphere where partici-

pants should move back after touching a fruit was visible for a random time interval between 0.4 and 0.6 s. This random dwelling time was selected to avoid that participants would anticipate the appearance of a new fruit, and thus, allowed us to detect more precisely the time between a new fruit appeared and the initiation of the movement (movement onset). The green sphere also appeared when starting a new block.

The blue and green spheres had a diameter of 4 cm and, when the blue sphere was in contact with the green one, the size of the green sphere increased by 10% to offer visual feedback and increase tolerance to small hand displacements. To detect the contact between fruits and the blue sphere, the orange and apples had spherical colliders mapped to their shape with diameters of 10 cm and 7.52 cm, respectively. The lower part of the pear was mapped by a spherical collider with a diameter of 5.78 cm and a capsule-like collider with a height of 7.31 cm and a diameter of 2.38 cm. All these dimensions were chosen so the whole workspace would fit within the visualization technology with the smallest field of view, i.e., the Meta 2 with a diagonal field of view of 90°.

The participants performed a cognitive task in parallel to the motor task. They were asked to count out loud the number of fruits separately for each fruit category (orange, apple, and pear). They were instructed not to move towards the fruit before starting to say the counting value. The participants started each block counting from zero. The appearance of the fruit categories were randomized with the only condition that each block should contain one fruit of each three categories, except for the first and last blocks, which only contained pears.

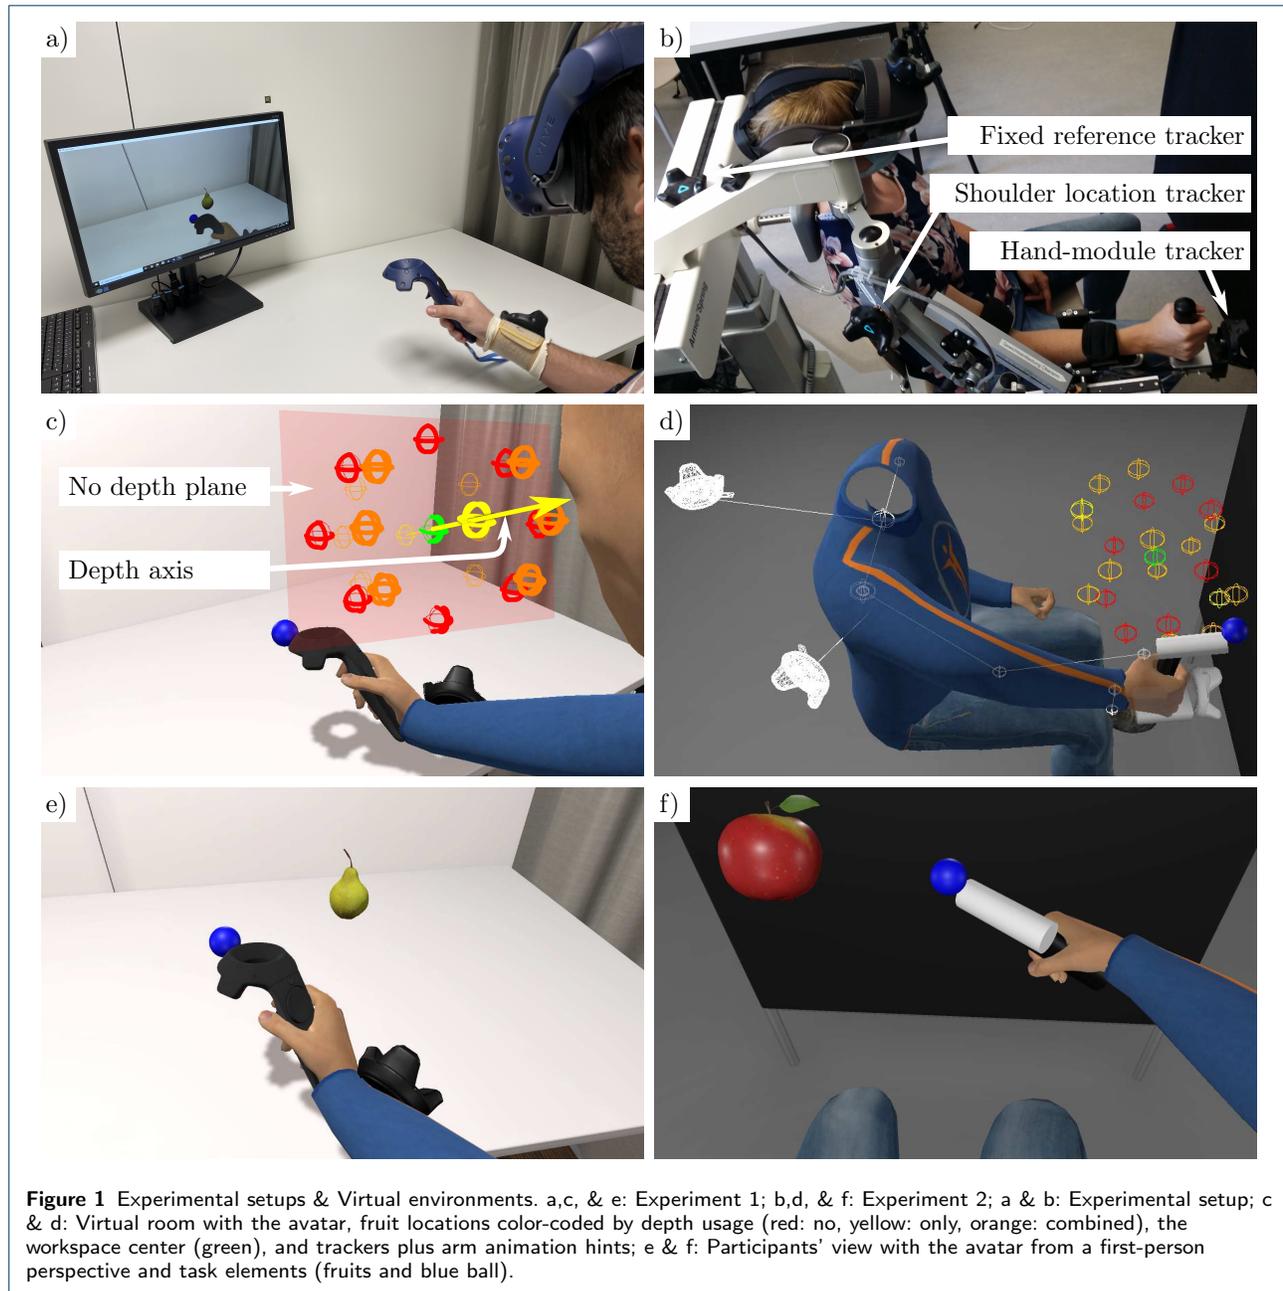

### Virtual Environment

The VE displayed in the 2D screen and IVR conditions was composed of a virtual representation of the room, including the walls, the ceiling with a lamp, the ground, the door, the curtain, and the table (Fig. 1 e). Respecting the physical light location, shadows were cast from the avatar, the virtual HTC Vive controller held in the right hand, and the virtual HTC Vive trackers on the arm. The blue sphere (touching point), green sphere (workspace center), and the fruits did not cast shadows as it was not possible to render those shadows

with the Meta 2 AR display and we wanted to have a fair comparison between technologies. In the AR condition, only the spheres and fruits were rendered and lit by the same light sources used in the other VE. A black and unlit controller was also rendered on top of the real one for occlusion purposes; the default occlusion algorithm of the Meta 2 worked rather well for detecting participants' hands, but not the controller, probably due to its material.

The avatar's arm was animated with inverse kinematics (IK) using the tracked position and orienta-

tion of the controller held in the participant’s hand. Only in the IVR condition, the avatar’s neck and spine were animated with IK based on the orientation of the HMD. The whole avatar’s position was also adapted in the 3D space to match the tracked position of the HMD.

### Protocol

A visual representation of the experimental protocol is shown in Fig. 2, a. Each participant performed the same motor and cognitive tasks under the three different visualization technology conditions (IVR, AR, and 2D screen). The order of the conditions was balanced between all participants. In each visualization condition, we aimed at displaying a similar environment (i.e., experiment room), which required a similar interaction (i.e., moving in 3D with a tracked controller).

Before the experiment started, participants sat on a comfortable chair, answered the demographic questionnaire (see Table 1), and received the tasks instructions orally. Before each condition, a calibration of the corresponding visualization technology was performed (see section *Experimental Setup*). After all conditions were performed, participants filled in the following questionnaires: The “Raw Task Load Index” (RTLX [32]) to evaluate the subjectively reported cognitive load (with subscales “Mental Demand”, “Physical Demand”, “Temporal Demand”, “Performance”, “Effort”, and “Frustration”); several items from the “Intrinsic Motivation Inventory” (IMI [33]) to measure the motivation (with subscales “Interest/Enjoyment”, “Perceived Competence”, “Effort/Importance”, and “Pressure/Tension”); and the “System Usability Scale” (SUS [34]) to evaluate the system usability.

The questionnaires were answered on a computer using REDCap electronic data capture tool [35] hosted at the University of Bern, Switzerland. For each question, three lines of answers were possible – one per visualization condition, respecting the order of appearance of each display. The SUS and IMI were answered using a Likert scale between 1 and 7 points; 1 indicating “Not at all”, 4 indicating “Somewhat true”, and 7 indicating “Very true”. The RTLX used a markless slider without numerical values with 100 encoded intervals. All questions were translated into German.

### Data Processing

**Questionnaires.** A single score was computed for the SUS questionnaire by averaging all questions and rescaling from the original 1-7 likert scale to 0-100. For the IMI, a single value per subscale was computed by averaging all the questions within each subscale, 5-7 questions per subscale. For the RTLX, we used the

selected values on the markerless slider (from 0-100) for the six questions, one question per subscale.

**Cognitive Task.** For the counting task, a score was computed for each block as the percentage of correct counted fruits over the total of presented fruits in that block. If a mistake was made while counting a fruit, participants could continue counting from this erroneous value – i.e., if the expected number was three, but the participant said four, both four or five would be considered as a correct next counting value. The percentages calculated for each of the eight blocks within a condition were averaged into a single value for each participant.

**Movement Quality.** The position and orientation of the HTC controller were recorded at an approximate frequency of 500 Hz. The data was cut into individual fruit-reaching movements, starting from the instant that the green sphere disappeared and the fruit appeared and ending when the fruit disappeared, i.e., when the blue sphere collided with the fruit collider.


Four movement quality metrics were computed from the blue ball location to evaluate the movement quality: (1) The **normalized movement duration** (s/m), defined as the duration of the reaching movement divided by the minimum distance between the last and first position within the movement; (2) The **trajectory straightness ratio** (n.u.), defined as the length of the path followed divided by the minimum distance between the last and first position within the movement; (3) The **peak velocity** (m/s) defined as the highest velocity value during the movement; and (4) The **number of velocity peaks** – reflecting the movement smoothness [36].

We also calculated the **movement onset**, defined as the time lapsed between the disappearance of the green sphere and the instant the speed of the blue sphere reached the threshold of 0.2 m/s.

The data were processed in Python *Python* 3.7.9, with the packages *numpy* 1.20.2, *pandas* 1.1.3, *quaternion* 2021.4.5.14.42.35, and *scipy* 1.5.2.

### Statistical Analyses

As we expected that the quality of the reaching movements requiring depth would decline in the 2D screen condition, we classified the reaching movements within three categories, based on the fruit location (**depth usage**): (1) *no depth*, i.e., only movements along the horizontal and/or vertical axes were needed; (2) *depth only*, i.e., no required movements along the horizontal nor the vertical axes were needed; and (3) *combined depth*, i.e., the fruit location required movements in the depth axis along with the horizontal and/or vertical axes.

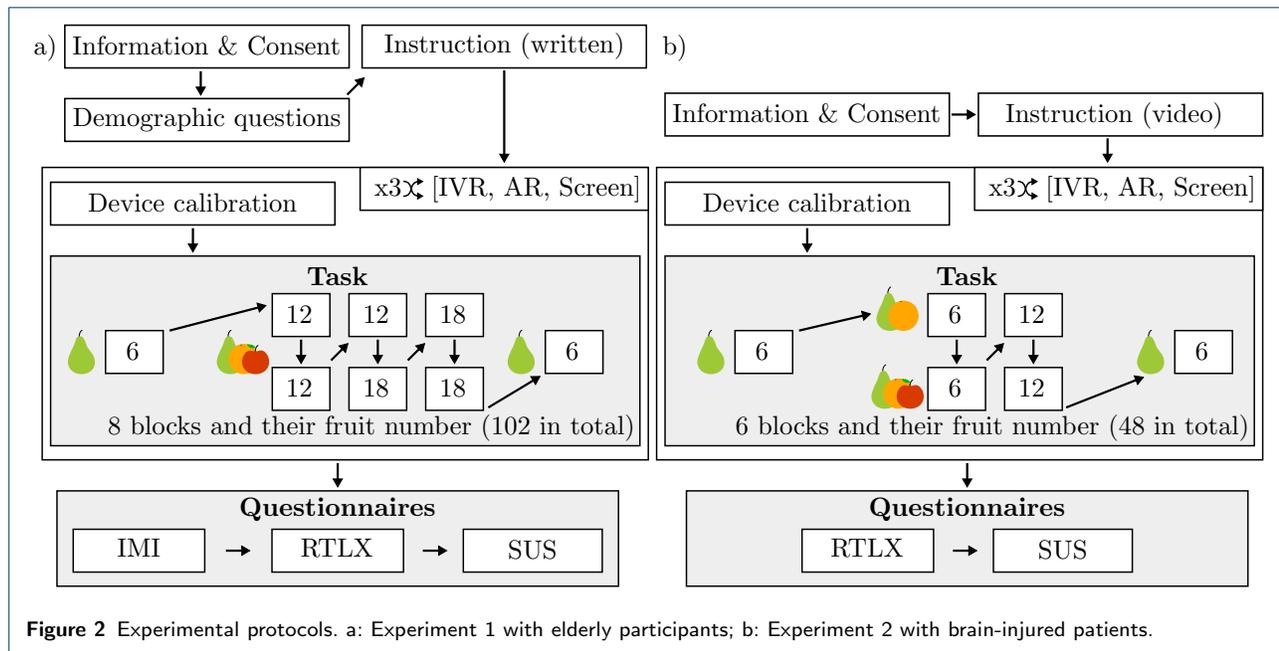

**Figure 2** Experimental protocols. a: Experiment 1 with elderly participants; b: Experiment 2 with brain-injured patients.

To investigate the impact of the *visualization technology* (IVR, AR, 2D screen) and the *depth usage* (no depth, depth only, combined depth) and their interaction on the four movement quality metrics and movement onset, we performed a two-way 3 x 3 RM-ANOVA. None of the movement quality metrics followed a normal distribution, based on Kolmogorov-Smirnov tests. However, in the absence of non-parametric alternatives, we decided to use the RM-ANOVA knowing that our analyses were, therefore, more conservative than non-parametric tests.

To investigate the impact of the visualization technology on the motivation (IMI) and reported cognitive load (RTLX), we computed an averaged value per subscale, following each specific questionnaire convention. For each questionnaire, we performed a one-way repeated-measures multivariate analysis of variance (RM-MANOVA) considering the visualization technology as an independent variable and the subscales of the questionnaires as dependent variables. For the system usability (SUS), as it has no defined subscales, we performed a one-way repeated-measures analysis of variance (RM-ANOVA) on the average of all questions. Only the IMI had one extreme outlier ( $outlier < Q_1 - 3 \cdot IQR$  or  $outlier > Q_3 + 3 \cdot IQR$ ;  $Q_1$ : first quartile,  $Q_3$ : third quartile, and  $IQR = Q_3 - Q_1$ ). Removing this participant and performing the RM-MANOVA again led to similar results, therefore, the reported values include this participant.

To analyze the impact of the visualization technology on the counting accuracy – the objective measure of cognitive load –, we ran a Friedmann’s test as the

Kolmogorov-Smirnov test indicated a normality violation for the counting accuracy in IVR.

When a significant main effect of a factor or an interaction was found, post-hoc pairwise *t*-tests were performed. We applied the Greenhouse-Geisser sphericity correction for factors violating the sphericity assumptions in the RM-MANOVA and RM-ANOVA tests. The reported effect sizes for the RM-MANOVA and RM-ANOVA tests are the partial  $\eta^2$ . We reported the Cohen’s D for the post-hoc tests, and for the Friedmann’s test, the Kendall’s coefficient of concordance (W).

Three participants (two females, one male) were excluded from the statistical analyses. For two participants, we encountered technical problems with the AR HMD device. The third exclusion was due to the inability of the participant to stay in contact with the green sphere between each fruit reach in the 2D screen condition. For each metric, we excluded extreme outliers ( $< Q_1 - 3 \cdot IQR$  or  $> Q_3 + 3 \cdot IQR$ ;  $Q_1$ : first quartile,  $Q_3$ : third quartile, and  $IQR = Q_3 - Q_1$ ). Over the total of 5886 reaching movements performed by the 17 participants in all visualization conditions, the extreme outliers removal led to 660 movements removed from the movement onset computation (IVR: 164, AR: 230, 2D screen: 266; 280 of them did not reach the minimum velocity threshold), 140 from the normalized movement duration (IVR: 55, AR: 56, 2D screen: 29), 135 from the trajectory straightness ratio (IVR: 35, AR: 72, 2D screen: 28), 51 from the peak velocity (IVR: 9, AR: 14, 2D screen: 28), and 174 from

the number of velocity peaks (IVR: 43, AR: 83, 2D screen: 48).

The RM-MANOVAs and their univariate follow-up tests were performed in *SPSS* version 27. The RM-ANOVAs and the post-hoc tests were performed using *Python* 3.7.9, with the packages *numpy* 1.20.2, *pandas* 1.1.3, *r-afex* 0.23.0, *r-effsize* 0.7.6, *rpy2* 2.9.4, *scipy* 1.5.2, and *statsmodels* 0.12.2. The significance level was set to  $\alpha = 0.05$  for all statistical tests.

## Experiment 2 - brain-injured Patients

### *Participants*

Five participants with moderate motor impairment due to a neurologic incident, in the subacute phase (< two months after the incident) and aged 36 to 69 ( $49.88 \pm 12.55$ ) participated in the second experiment. The clinical data of the participants can be found in table 2. They were recruited by therapists from the rehabilitation unit of the University Hospital Bern, Switzerland. Participants provided written informed consent to participate in the study. The study was approved by the local Ethics Committee (ref.: 2017-02,195) and conducted in compliance with the Declaration of Helsinki. Participants did not receive any compensation for their participation in the study.

### *Experimental Setup & Virtual Environments*

Since patients suffered moderate motor impairments, we adapted the fruit-reaching motor task so the VR task could be interfaced with the Armeo®Spring (Hocoma, Switzerland) to provide arm weight support during the experiment. The weight support system and VR game interfaced using User Datagram Protocol (UDP) communication, which was provided by Hocoma, Switzerland. The task was implemented to be feasible both with the left or right arm, so patients could always perform it with their paretic arms.

We noticed that the hand/device end-effector position obtained by the UDP communication from the ArmeoSpring – calculated from the device position sensors – was not precise enough, i.e., there was a visible offset between the real hand position and the one rendered in AR using the device forward kinematics calculations. To reduce this visual mismatch, we included three *HTC Vive trackers* (2018) to track several links of the mechanical structure. A first tracker was placed on the height-adjustable part of the ArmeoSpring, which is used to adjust the height of the device based on the patient’s height and is fixed during the training (Fig. 1, b; fixed reference tracker). Its location was, therefore, considered as a fixed reference frame to our system, from which we were able to compute the patient’s seated position (assuming a fixed position shift from the tracker to the closest point

between the two shoulders, visible in Fig. 1, d). The second tracker was placed on the ArmeoSpring upper arm link at the shoulder level to track the location of the patient’s shoulder. This was needed as the device allows shoulder movements on the sagittal plane, but does not incorporate sensors to measure those. Finally, the third tracker was mounted with an in-house 3D-printed fixation element on the ArmeoSpring hand module to track the patient’s hand location. The avatar’s arm was then animated using the *Unity* plugin *FinalIK* v1.9. We used the tracker on the hand module to compute the hand position and the tracker next to the shoulder to compute the root position of the avatar. Finally, the elbow position was computed using the *FinalIK* algorithm with the UDP ArmeoSpring sensor data as a hint for the elbow location.

To facilitate the recruitment of brain-injured patients, the experiment was performed in a room at the University Hospital Bern (Inselspital), different than the one used in the first experiment, which was performed at the Swiss Institute for Translational and Entrepreneurial Medicine (SITEM-Insel). The room had artificial and controllable lighting. To remove background details that could interfere with the visibility of the fruits in the AR condition, a black board was placed in front of the participants and behind the task workspace. The virtual reproduction of the room included only four walls, the ceiling, the ground, and the black background board (Fig. 1 f). The virtual light source within the VE used the same location as the real one and was also employed to compute the lighting on the virtual elements in the AR modality. No calibration was needed for the 2D screen modality.

The avatar rendered in the IVR and 2D screen conditions held a vertical black cylinder (corresponding to the real ArmeoSpring hand module; Fig. 1 f). In all conditions (also in AR), a white virtual horizontal cylinder was added to the hand module. A virtual blue sphere of 4 cm in diameter was attached at the end of this white cylinder. This virtual element was included to preserve the distance from the patient’s hand location and the touching point in Experiment 1 due to the length of the HTC Vive controller.

### *Protocol & motor and Cognitive Tasks*

The protocol of Experiment 2 is depicted in Fig. 2, b. The protocol was similar to the one described in Experiment 1, with only minor differences to reduce the duration and task difficulty. First, there was no demographic questionnaire at the start of the experiment, as the most relevant information (Table 2) was provided by the therapists with the patient’s consent. Second, the oral instructions were supported with a video to show the task to be performed and the different visualization conditions. Third, the AR calibration step

**Table 2** Patients' characteristics

#	Gender	Age	Lesion type	Lesion location	Time since onset (days)	Sensori-motor hemiparesis side	Aphasia	Chedoke McMaster Hand assessment score <sup>1</sup>	Neuropsychological deficits
1	Female	36	Hemorrhagic stroke	Paracentral left	34	Right	No	5	Reduced digital span and verbal fluency
2	Male	38	Epilepsy surgery	Resection of the right operculum	28	Left	No	7	Attention, visuo-constructive, and executive deficits
3	Male	69	Ischemic stroke	Right frontoparietal	48	Left	No	5	Left hemineglect
4	Male	58	Hemorrhagic stroke	Left basal ganglia	35	Right	Yes	4	Attention and executive deficits. Reduced resilience
5	Male	48	Ischemic stroke	Arteria cerebri media right	33	Left	No	4	Left hemineglect, dysexecutive symptoms, perseveration, visuo-constructive disturbances

<sup>1</sup> Test performed within one week before or after the experiment

was not performed because the therapists and medical doctors considered it too demanding for the neurologic patients. Fourth, to shorten the whole experiment, we did not include the motivation questionnaire, as it was the longest questionnaire. The scale of the usability questionnaire was changed from a 7-point to a 5-point Likert scale. Finally, to facilitate the understanding of the cognitive load and usability questionnaires (RTLX & SUS), those were provided in paper form – instead of using REDCap in a computer. We included photos of the different displays to help identifying the different conditions and, when needed, the assistance of the experimenter was provided. The order of the questionnaires was balanced between the patients, and the order of the items within each questionnaire was randomized for each patient.

The motor and cognitive tasks were very similar to the ones performed in Experiment 1, with three exceptions. First, we adjusted the difficulty of the tasks by adding only six blocks of, respectively, 6, 6, 6, 12, 12, and 6 fruits, i.e., a total of 48 fruits per condition. The first and last blocks only contained pears, the second and fourth blocks only contained pears and oranges, and the third and fifth block contained the three fruit categories. Second, the diameter of the green sphere was increased from 4 cm to 5 cm to be more tolerant to errors. Third, the workspace had the same size but its center was centered on the left-right axis, and located 31 cm down, and 40 cm away from the participants' eyes to fit a space easily reachable by the patients.

#### Data Processing

A single score, rescaled from the original 1-7 likert interval to 0-100, was computed for the SUS by averaging all the questions. For the RTLX, we used an analogical

scale of 122-125.5 mm (variations due to printers inconsistency) with 21 interval marks. The value of each RTLX answer was calculated as the distance from the left border to the centers of the participants' added responses (crosses) over the analogical scale (rounded to the closest 0.5 mm), divided by total physical scale size – i.e., 122-125.5 mm – and multiplied by 100. We used the same procedure as in Experiment 1 to compute the cognitive task score.

We computed the same four movement quality metrics and the movement onset for each (fruit) reaching movement as in Experiment 1, using the recorded position and rotation of the hand module tracker. We categorized the movements using the same depth usage classification as in Experiment 1.

We followed the same procedure to find and remove movement outliers. Over the total of 720 individual reaching movements, the outliers removal led to 164 movements removed from the movement onset computation (IVR: 46, AR: 48, 2D screen: 70; 144 of them did not reach the minimum speed threshold), 15 from the normalized movement duration (IVR: 8, AR: 4, 2D screen: 3), three from the trajectory straightness ratio (IVR: 1, AR: 1, 2D screen: 1), six from the peak velocity (IVR: 2, AR: 1, 2D screen: 3), and 14 from the velocity peaks number (IVR: 4, AR: 3, 2D screen: 7).

As the number of patients was relatively low, we did not have enough statistical power to perform statistical analyses. Therefore, we only report the mean and standard deviation for each metric.

## Results

### Experiment 1: Healthy Elderly Participants

The results of the RM-MANOVAs, RM-ANOVAs, and Friedmann's tests for the self-reported questionnaire

values – i.e., motivation (IMI), cognitive load (RTLX), and usability (SUS) –, the movement quality metrics – i.e., normalized movement duration, trajectory straightness ratio, peak velocity, and velocity peaks number –, the movement onset, and the counting accuracy can be found in Table 3. The results of the follow-up analyses are summarized in Table 4. The impact of the visualization technology on the different metrics is graphically represented in Fig. 3 and the interaction effect between the visualization technology and the depth usage on movement quality and movement onset in Fig. 4.

**Table 3** Experiment 1 results from the RM-MANOVAs on the effect of the visualization technology (*Vis. Tech.*) on the questionnaire data, the results from the RM-ANOVAs on the effect of the visualization technology, depth usage (*Depth*) and its interaction (*Vis. Tech.:Depth*) on the movement quality and movement onset, and the Friedmann's test on the counting accuracy. For the RM-MANOVAs, the reported  $F$  values are the Wilks  $\lambda$

Effect	df	F	Effect size	Sig.
<i>RM-MANOVA - Motivation (IMI)</i>				
Vis. Tech.	4	.79	.41	.627
<i>RM-MANOVA - Cognitive Load (RTLX)</i>				
Vis. Tech.	6	.66	.61	.745
<i>RM-ANOVA - Usability (SUS)</i>				
Vis. Tech.	2	2.42	.95	.105
<i>RM-ANOVA - Normalized Duration</i>				
Vis. Tech.	2	26.4	.7	< .001 *
Depth	2	11.28	.83	.003 *
Vis. Tech.:Depth	4	9.0	.84	.003 *
<i>RM-ANOVA - Trajectory Straightness Ratio</i>				
Vis. Tech.	2	12.43	.74	< .001 *
Depth	2	14.98	.94	.001 *
Vis. Tech.:Depth	4	18.54	.94	< .001 *
<i>RM-ANOVA - Peak Velocity</i>				
Vis. Tech.	2	7.0	.78	.012 *
Depth	2	6.17	.98	.016 *
Vis. Tech.:Depth	4	2.39	.97	.12
<i>RM-ANOVA - Velocity Peaks Number</i>				
Vis. Tech.	2	24.97	.68	< .001 *
Depth	2	9.88	.65	.005 *
Vis. Tech.:Depth	4	4.98	.73	.012 *
<i>RM-ANOVA - Movement Onset</i>				
Vis. Tech.	2	11.21	.61	.003 *
Depth	2	8.29	.64	.01 *
Vis. Tech.:Depth	4	3.49	.61	.07 •
Effect	df	$\chi^2(2)$	Effect size	Sig.
<i>Friedmann's test - Counting accuracy</i>				
Vis. Tech.	2	.27	.008	.874

\*  $p < 0.05$ , •  $p < 0.1$

### Movement Quality

With the IVR technology, elderly healthy participants performed movements of shorter duration compared to the other two visualization technologies (Fig. 3 a). Visualizing the movements in IVR also resulted in straighter, faster, and smoother movements (i.e., less number of velocity peaks) than with the 2D screen (Fig. 3 b-d). With AR, the reaching movements were of

shorter duration, straighter, and smoother compared to the 2D screen (Fig. 3 a,b,d).

Movements that required moving along the depth axis (either only along the depth axis or in combination with another dimension) were in general of longer duration, less straight, and less smooth than movements that did not incorporate depth at all (Table 4). Furthermore, movements that only required moving along the depth axis were also of longer duration, less straight, and less smooth than movements combining depth with another dimension.

We also found significant interaction effects between the visualization technology and the depth usage in all movement quality metrics, except in the number of velocity peaks (Table 3). Post-hoc tests revealed that, for the 2D screen, the reaching movements were of shorter duration, straighter, and smoother when there was no depth component compared to the combination of depth with another dimension (Table 4, Fig. 3). The movements were also straighter when no depth was used compared to movements along only the depth axes (Fig. 3 b). When comparing the same depth usage between different technologies, we found that when no depth was used, IVR led to shorter duration and smoother movements than the 2D screen and a trend also indicated that they were of shorter duration than with AR (Fig. 3 a,d). When only depth was used, both HMDs led to shorter duration and straighter movements than the 2D screen (Fig. 3 a,b). The 2D screen also led to less straight movements than IVR and a trend indicated less straight movements than AR (Fig. 3 b).

### Movement Onset

With the IVR HMD, participants performed reaching movements towards the fruits that started earlier compared to the two other technologies – i.e., smaller movement onset (Fig. 3 e). With AR, the movements also started earlier compared to the 2D screen.

The onsets of reaching movements requiring only the depth dimension were longer than those movements that combined depth with another dimension, or not using depth at all (Table 4).

We found that the interaction effect between the visualization technology and the depth usage in the movement onset did not reach significance ( $p = 0.07$ ; Table 3). Nevertheless, we decided to run post-hoc tests to have a closer look at potential differences (Table 4). Post-hoc tests revealed that when comparing different depth usages within the same visualization technology, there was a trend within the IVR technology, indicating that movements using only depth started later than the ones combining depth with another dimension. Within the same depth usage, we

**Table 4** Experiment 1 results from the post-hoc tests. Visualization technologies: IVR, AR, 2D screen. Depth usage: No (movements along the horizontal and/or vertical axes), Only (movements only along the depth axes), Combined (movements in the depth axis along with the vertical and/or vertical axes)

Group1	Group2	T	Effect size	Sig.
<b>Normalized Duration</b>				
IVR	AR	-3.47	.61	.009 *
IVR	2D screen	-5.87	.94	< .001 *
AR	2D screen	-4.83	.77	.001 *
Combined	No	3.31	-.33	.013 *
Combined	Only	-3.04	.31	.023 *
No	Only	-3.34	.58	.012 *
AR & Combined	2D screen & Combined	-5.39	.97	.002 *
AR & Only	2D screen & Only	-4.24	.69	.022 *
2D screen & Combined	2D screen & No	4.97	-.53	.005 *
2D screen & No	2D screen & Only	-3.62	.67	.082 ●
IVR & Combined	2D screen & Combined	-6.63	1.16	< .001 *
IVR & No	AR & No	-3.57	.57	.093 ●
IVR & No	2D screen & No	-4.96	.68	.005 *
IVR & Only	2D screen & Only	-4.63	.89	.01 *
<b>Straightness ratio</b>				
AR	2D screen	-3.15	.67	.019 *
IVR	2D screen	-4.91	.79	.001 *
Combined	No	4.03	-.22	.003 *
Combined	Only	-2.86	.24	.034 *
No	Only	-4.11	.41	.003 *
AR & Only	2D screen & Only	-4.86	.82	.006 *
2D screen & Combined	2D screen & No	6.04	-.47	.001 *
2D screen & No	2D screen & Only	-5.05	.59	.004 *
IVR & Combined	2D screen & Combined	-5.75	.92	.001 *
IVR & Only	2D screen & Only	-5.12	.9	.004 *
<b>Peak Velocity</b>				
IVR	2D screen	5.23	-.92	< .001 *
No	Only	-2.82	.22	.037 *
<b>Velocity Peaks Number</b>				
AR	2D screen	-6.52	1.12	< .001 *
IVR	2D screen	-5.52	1.25	< .001 *
Combined	No	3.62	-.63	.007 *
Combined	Only	-2.73	.35	.045 *
No	Only	-3.19	.79	.017 *
AR & Combined	2D screen & Combined	-7.72	1.44	< .001 *
AR & No	2D screen & No	-4.59	1.09	.011 *
AR & Only	2D screen & Only	-3.85	.79	.051 ●
2D screen & Combined	2D screen & No	4.44	-.88	.015 *
IVR & Combined	2D screen & Combined	-5.86	1.67	.001 *
IVR & No	2D screen & No	-4.49	.87	.013 *
IVR & Only	2D screen & Only	-3.87	.77	.049 *
<b>Movement Onset</b>				
IVR	AR	-3.73	.46	.005 *
IVR	2D screen	-3.71	.67	.006 *
AR	2D screen	-3.03	.52	.024 *
Combined	Only	-3.4	.58	.011 *
No	Only	-3.22	.8	.016 *
IVR & Combined	IVR & Only	-3.66	.41	.076 ●
IVR & Combined	AR & Combined	-4.01	.37	.036 *
IVR & Combined	2D screen & Combined	-3.75	.73	.063 ●


\*  $p < 0.05$ , ●  $p < 0.1$

found that, for locations combining depth with another dimension, IVR led to movements starting earlier than AR and a trend indicated that they started earlier than the 2D screen (Fig. 4 e).

#### Counting Task Accuracy and Questionnaires

The overall reported usability was high (>80 over a maximum of 100) with every visualization technology and did not differ significantly across them (Fig. 3 h).

The reported motivation was also relatively high (>4.5 over a maximum of 7) – considering the fact that the task was not designed to enhance motivation – and did not differ significantly across visualization technologies (Fig. 3 i). The self-reported cognitive load – measured with the RTLX questionnaire – did not differ significantly across visualization technologies (Fig. 3 g). We did not find significant differences either in the counting accuracy in the parallel cognitive task,

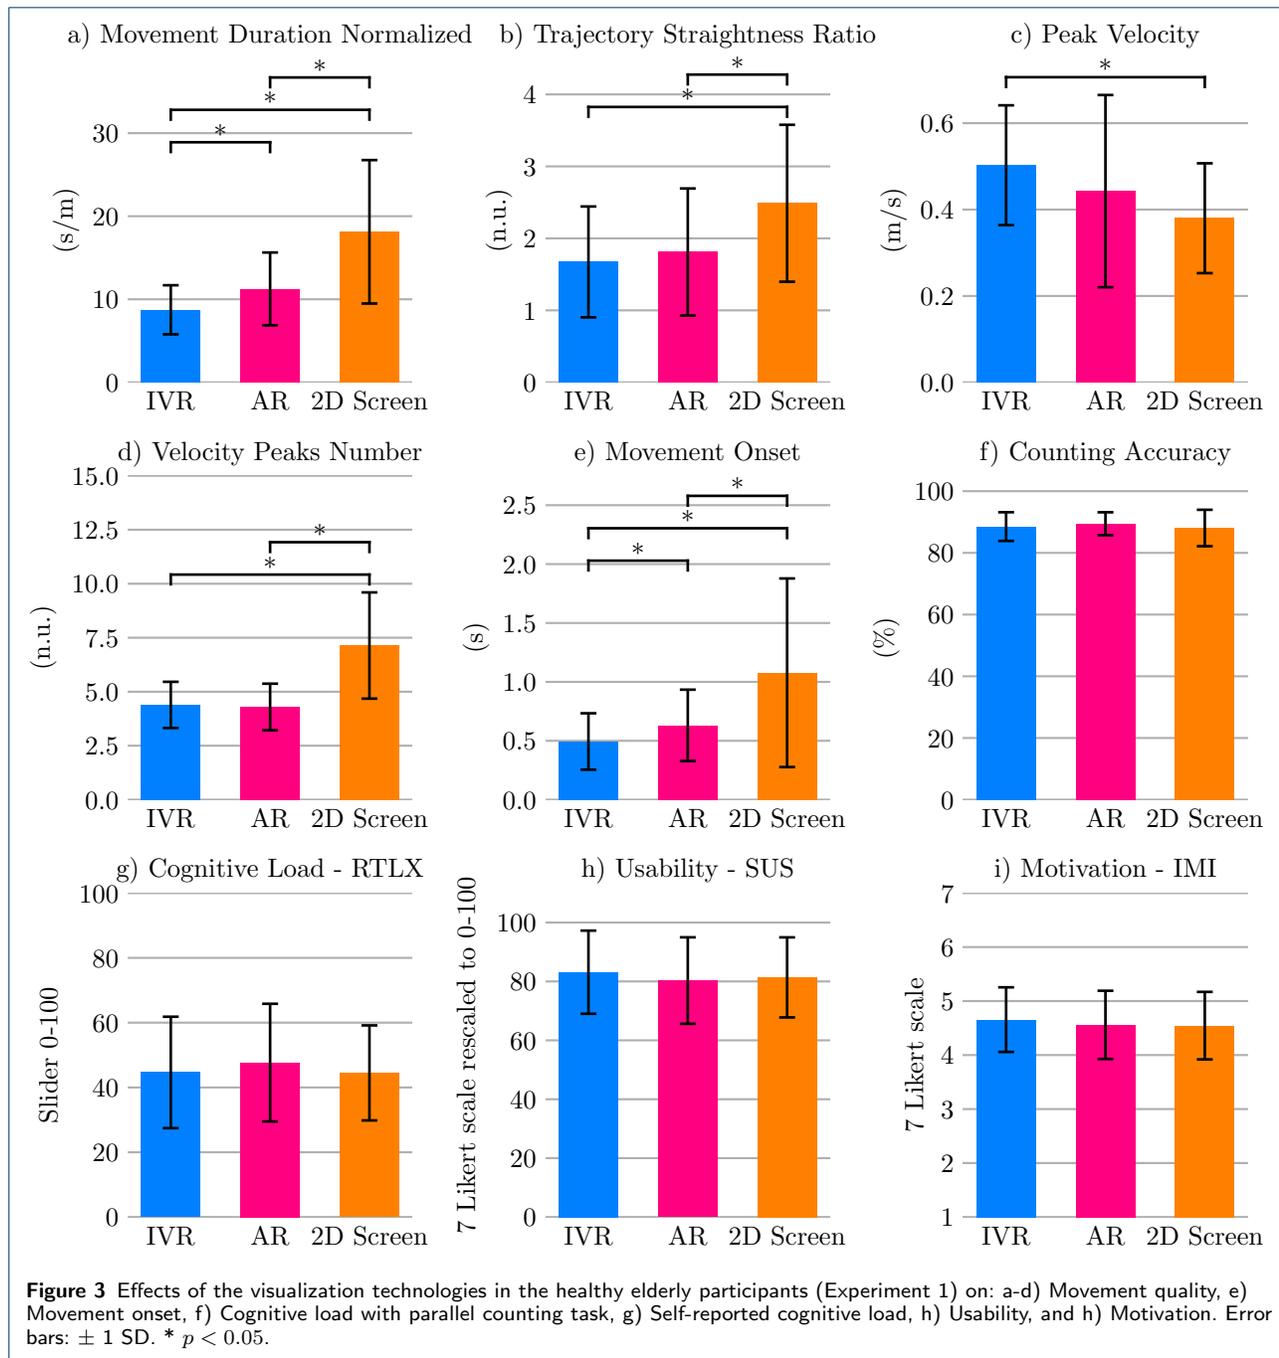

which remained high across technologies ( $>80$  over a maximum of 100) (Fig. 3 f).


### Experiment 2: Brain-injured Patients

A summary of the descriptive statistics of the movement quality metrics, movement onset, counting task accuracy, self-reported cognitive load (RTLX), and usability (SUS) under the three different visualization technologies can be found in Table 5 and a graphical representation is available in Fig. 5. The interaction

between the visualization technology and the depth usage on the movement quality and movement onset can be found in Table 6 and a graphical representation is available in Fig. 6.

### Movement Quality

We observed that both IVR and AR HMDs seemed to lead to shorter duration, straighter, and smoother movements compared to the 2D screen (Fig. 5). Another interesting observation was that the standard

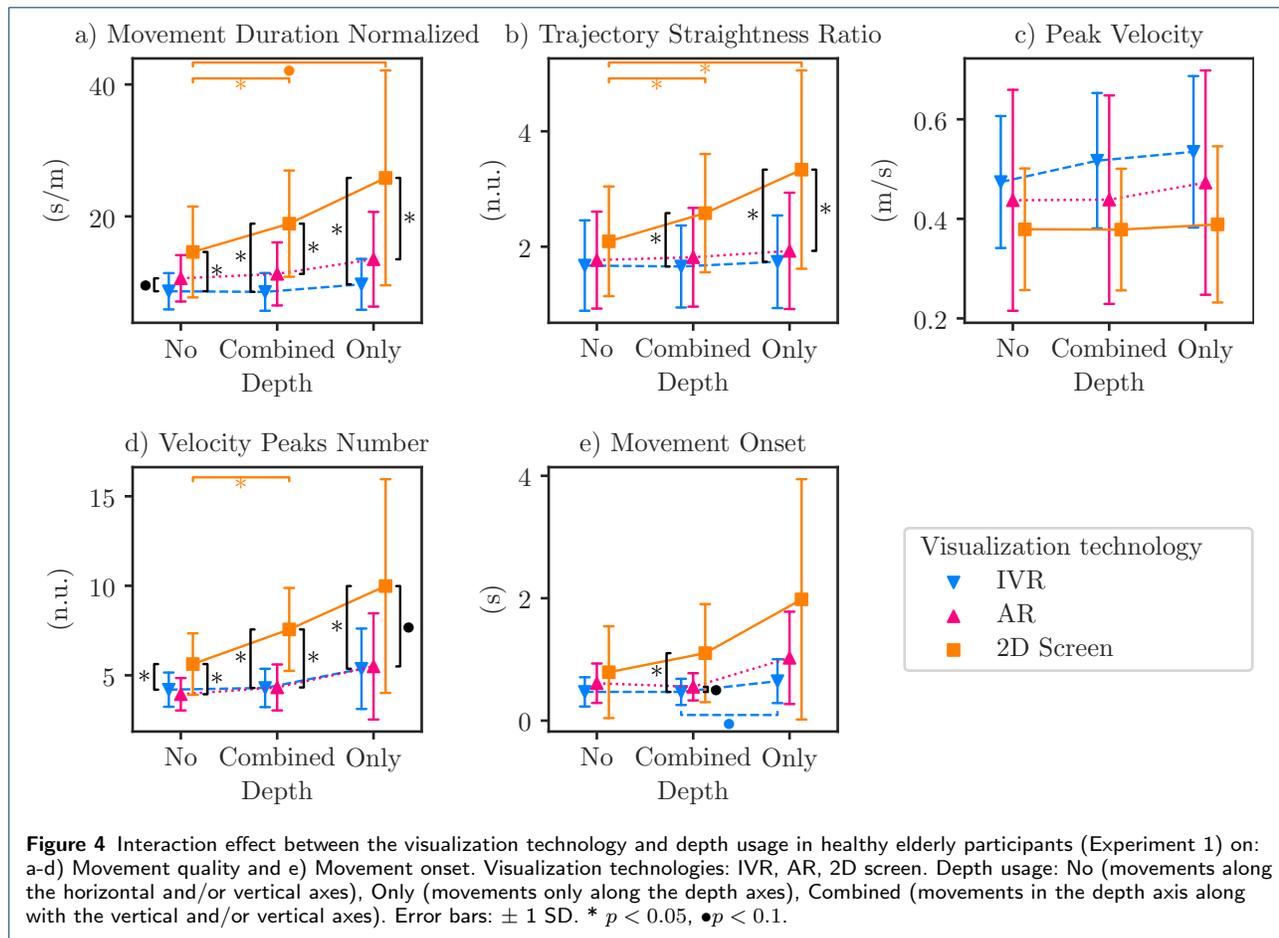

deviation of those metrics was much smaller with the HMDs than with the 2D screen. The reaching movements seemed also to reach higher velocity peaks with both HMDs compared to the 2D screen, but the differences in this specific metric seemed smaller than in the other movement quality metrics.

Regarding depth usage (Fig. 6), similar to what we observed in the elderly participants, only the 2D screen seemed to elicit longer duration, less straight, and less smooth movements when the reaching towards fruits did not require moving in the depth axis compared to movements requiring no depth. None of the HMDs seemed to be impacted by depth usage. As with the healthy elderly participants, there seemed to be no interaction effect on the peak velocity, although we observed a slight decrease in the peak velocity in the 2D screen when moving in the depth axis was required, which was not observed in the HMDs.

#### Movement Onset

We observed that both HMDs seemed to lead to smaller movement onsets with smaller standard deviations compared to the 2D screen (Fig. 5 e). No dif-

ferences in the movement onset were, at first glance, observed between the AR and IVR visualizations. We also observed that the movement onset was larger when the reaching movements required moving in the depth axis (compared to no depth) only with the 2D screen (Fig. 6 e).

#### Counting Task Accuracy and Questionnaires

For the counting task accuracy, no apparent differences were observed between visualization technologies (Fig. 5 f). However, the reported cognitive load in the RTLX questionnaire seemed to be higher with the 2D screen than with the HMDs (Fig. 5 g). The self-reported cognitive load also seemed to be smaller with the IVR compared to the AR. Finally, regarding the usability, IVR was reported as the most usable, with a remarkable high value of 83, even higher than the average value reported by the elderly participants (Table 5, Fig. 5 h). The AR and the 2D screen visualizations showed a lower usability with a high between-subject standard deviation.

**Table 5** Descriptive statistics across visualization technologies in Experiment 2. Mean values and standard deviations of the movement quality, movement onset, cognitive load with a parallel task, self-reported cognitive load, and usability across visualization technologies for the brain-injured patients.

Variable	IVR	AR	2D Screen
Movement Duration Normalized (s/m)	11.99 ( $\pm 1.73$ )	12.6 ( $\pm 1.1$ )	19.39 ( $\pm 7.89$ )
Trajectory Straightness Ratio (n.u.)	1.58 ( $\pm 0.19$ )	1.58 ( $\pm 0.17$ )	1.98 ( $\pm 0.3$ )
Peak Velocity (m/s)	0.29 ( $\pm 0.06$ )	0.28 ( $\pm 0.06$ )	0.26 ( $\pm 0.06$ )
Velocity Peaks Number (n.u.)	4.92 ( $\pm 1.41$ )	4.83 ( $\pm 0.97$ )	8.72 ( $\pm 4.79$ )
Movement Onset (s)	0.87 ( $\pm 0.18$ )	0.93 ( $\pm 0.1$ )	1.58 ( $\pm 0.87$ )
Counting Accuracy (%)	95.83 ( $\pm 4.17$ )	93.33 ( $\pm 5.78$ )	93.75 ( $\pm 4.89$ )
Cognitive Load - RTLX <sup>1</sup>	22.81 ( $\pm 22.5$ )	26.35 ( $\pm 22.21$ )	29.95 ( $\pm 26.02$ )
Usability - SUS <sup>2</sup>	83.0 ( $\pm 13.62$ )	69.5 ( $\pm 25.15$ )	68.5 ( $\pm 27.7$ )

<sup>1</sup> Slider 1-100<sup>2</sup> 7 Likert scale rescaled to 0-100**Table 6** Descriptive statistics across visualization technologies and depth usage in Experiment 2. Mean values and standard deviations of the movement quality and movement onset across visualization technologies and depth usage for the brain-injured patients.

Variable	Visualization Technology	No Depth	Combined Depth	Only Depth
Movement Duration Normalized (s/m)	IVR	11.88 ( $\pm 1.59$ )	11.89 ( $\pm 1.9$ )	12.59 ( $\pm 2.52$ )
	AR	12.95 ( $\pm 2.29$ )	12.18 ( $\pm 1.36$ )	11.88 ( $\pm 2.98$ )
	2D Screen	15.89 ( $\pm 3.99$ )	20.94 ( $\pm 8.67$ )	25.4 ( $\pm 19.67$ )
Trajectory Straightness Ratio (n.u.)	IVR	1.5 ( $\pm 0.15$ )	1.63 ( $\pm 0.23$ )	1.52 ( $\pm 0.35$ )
	AR	1.63 ( $\pm 0.29$ )	1.57 ( $\pm 0.15$ )	1.35 ( $\pm 0.06$ )
	2D Screen	1.78 ( $\pm 0.18$ )	2.1 ( $\pm 0.42$ )	2.1 ( $\pm 0.97$ )
Peak Velocity (m/s)	IVR	0.29 ( $\pm 0.05$ )	0.3 ( $\pm 0.07$ )	0.28 ( $\pm 0.07$ )
	AR	0.28 ( $\pm 0.07$ )	0.29 ( $\pm 0.05$ )	0.29 ( $\pm 0.09$ )
	2D Screen	0.28 ( $\pm 0.07$ )	0.25 ( $\pm 0.05$ )	0.24 ( $\pm 0.05$ )
Velocity Peaks Number (n.u.)	IVR	4.33 ( $\pm 1.0$ )	5.37 ( $\pm 1.97$ )	4.97 ( $\pm 2.05$ )
	AR	4.8 ( $\pm 0.83$ )	4.92 ( $\pm 1.12$ )	4.45 ( $\pm 1.74$ )
	2D Screen	6.7 ( $\pm 1.52$ )	9.06 ( $\pm 5.66$ )	12.72 ( $\pm 16.03$ )
Movement Onset (s)	IVR	0.9 ( $\pm 0.25$ )	0.83 ( $\pm 0.21$ )	0.87 ( $\pm 0.19$ )
	AR	0.94 ( $\pm 0.14$ )	0.93 ( $\pm 0.09$ )	0.85 ( $\pm 0.32$ )
	2D Screen	1.24 ( $\pm 0.49$ )	1.72 ( $\pm 0.95$ )	1.88 ( $\pm 1.17$ )

## Discussion


In this study, we investigated whether IVR and AR HMDs could improve movement quality, reduce cognitive load, and increase motivation and usability compared to a 2D screen using parallel motor and cognitive tasks – i.e., reaching towards and counting virtual fruits, respectively – and questionnaires. We also analyzed whether the visualization technology impacted differently the movement quality and movement onset depending on the depth usage requirements of the reaching movements. We performed a first experiment with 20 elderly participants using a VR controller and a second pilot experiment with five brain-injured patients. For this second experiment, we adapted the experimental setup to be used in combination with a rehabilitation device (Armeo® Spring, Hocoma, Switzerland).

### HMDs Improve the Movement Quality

As hypothesized, the movement quality improved with HMDs compared to the 2D screen. The improvement in movement quality could be observed in all movement quality metrics, i.e., reaching with the HMDs resulted in shorter duration, faster, straighter, and smoother movements. The differences between HMDs and the 2D screen reached significance in the elderly

participants, while similar differences were observed in the smaller group of brain-injured patients. Contrary to our previous experiment with young healthy participants [23], AR showed a significant increase in the movement quality over the 2D screen in the elderly participants. The first observations in the patient population also seem to go in the same direction. Nevertheless, IVR still appears to surpass AR, as the movements were of shorter duration with IVR than with AR, at least in the elderly participants.


We expected that, only in the 2D screen condition, reaching movements would worsen when they involve the depth dimension – i.e., when the movements were only on the depth dimension or when they involved both horizontal/vertical movements together with the depth dimension. We expected that the depth dimension would be harder to visualize than the horizontal and vertical dimensions, which are directly mapped to the 2D screen plane. Our results confirm that, indeed, only in the 2D screen condition did the movement quality degrade when the depth dimension was required in the reaching movement (in terms of movement duration, straightness, and smoothness). The differences were more obvious between the movements with no depth vs. movements that required only moving in the

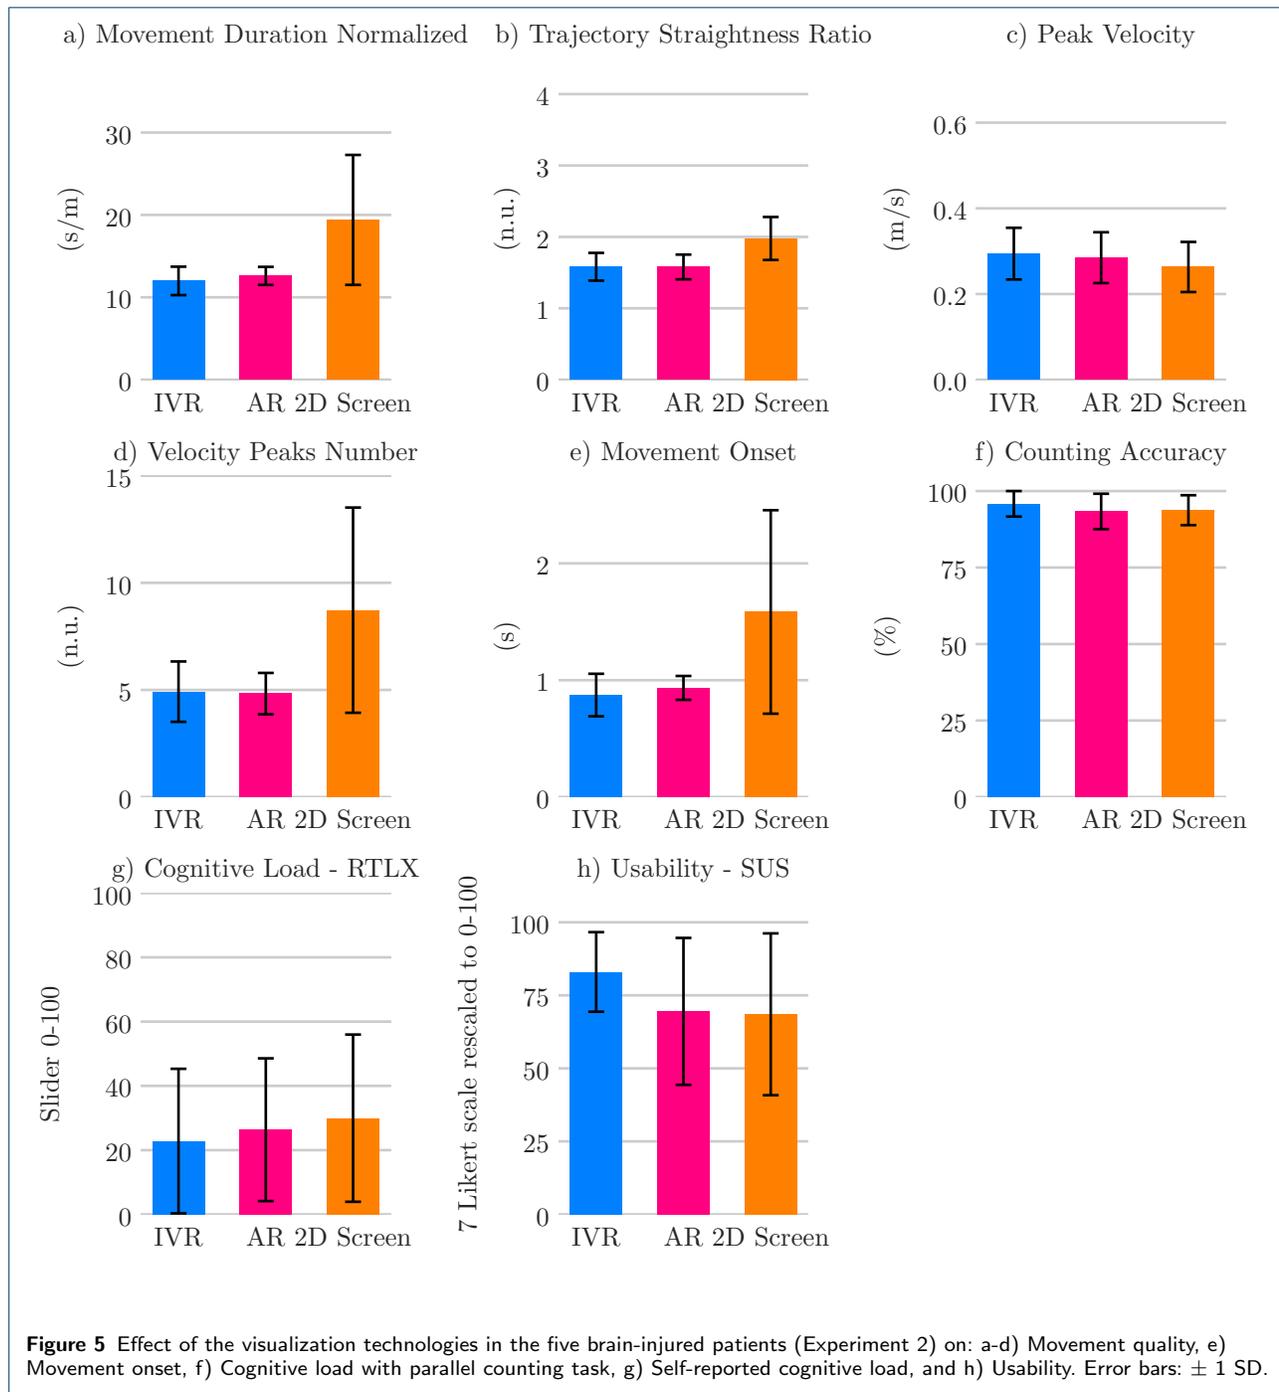

depth axes than vs. movements combining depth and the vertical/horizontal directions.

These analyses over the depth usage complete our previous “dimensionality” analyses with young healthy participants [23]. In our previous analyses, we compared the movement quality between visualization technologies based on the number of dimensions of the reaching movement, i.e., 1D, 2D, and 3D, instead of

the use of depth dimensions. For example, the “1D” movements contained movements not using the depth dimension but also some using it only. This might explain why we found more interaction effects between the visualization technologies and depth usage in the current study compared to those in the previous experiment. Our results differ from those of the study of Gerig et al. [25] where the quality of reaching move-

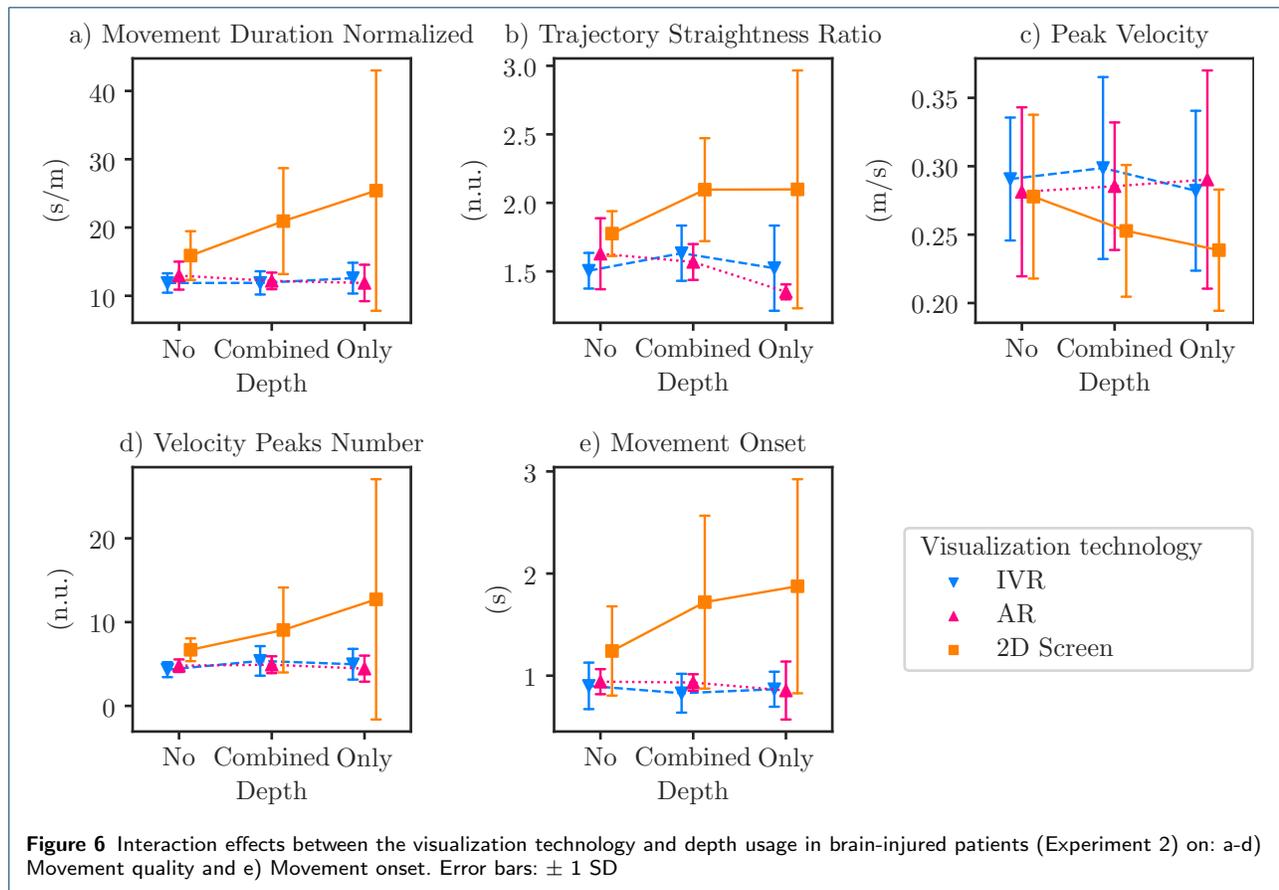

ments was compared between IVR and 2D screens. In their study with healthy participants, the authors reported shorter, straighter, and smoother movements in IVR than with a 2D screen with limited depth cues only when the 2D screen did not show a known-size object (i.e., the HTC controller) as an additional depth cue. In our experiment, the differences between modalities were significant, even if the controller was visually represented in the VE of both IVR and 2D screen modalities. However, we note that other depth cues (e.g., the shadows of the targets) were not present in our design as the selected optical see-through AR HMD could not render them, and we aimed to have a fair comparison between the technologies. Furthermore, in [25], the study population was also younger (18-40 y.o.) than our elderly population (64-89 y.o.) and, possibly, more cognitively fit.

Our results are encouraging for the adoption of HMDs into VR-based neurorehabilitation interventions. As identified by Palacios-Navarro and Hogan in their recent review [26], there is a lack of studies investigating how improved depth perception in immersive VR using HMDs could improve VR-based interventions in upper limb rehabilitation. In the real world,

many movements involve moving toward the depth direction, and therefore, it is important to train in an environment that alters as little as possible the perception and execution of such movements [6, 37, 19]. HMDs allow the provision of congruent sensory information between vision and proprioception, which – as observed in our experiment – enhances movement quality, but could also promote neuroplasticity by allowing meaningful movement training that promotes multi-sensory input to the central neural system [11]. Furthermore, this congruent sensory information might enhance skill transfer into ADL [6], as differences in depth perception might be associated with a low transfer of learned skills observed when training in non-immersive VR [38].

In the field of robotic rehabilitation, where the interaction with the rehabilitation system differs from real life, it is an open question whether patients relearn to use their arm or adapt to the training system (e.g., robotic device or visualization technology) [39]. Providing more naturalistic depth cues and reducing the visuospatial transformation with HMDs is a promising way to avoid the observed two-step learning in robotic VR-based interventions, where patients

first go through a first phase of learning how to use the system before focusing on their rehabilitation [20]. Therefore, the use of HMDs might allow patients to immediately train the targeted functional movements, gaining crucial rehabilitation time.

Finally, as movement quality metrics are used as indicators of patients' impairment level [40, 41], it is crucial that the technological rehabilitation solution minimizes its own impact on these metrics. Our study is a first step in that direction as we showed that HMDs allow participants to train movements with better quality, reducing the negative impact of the current technological solution using 2D screens on movement execution. Nevertheless, we note that in our experiments we did not compare the movements performed with either of the visualization technologies with reaching movements in the real world, as this has already been evaluated in previous literature (e.g., [21, 19, 22]).

#### HMDs Might Lower the Cognitive Load

We expected to observe a lower cognitive load with the HMDs compared to the 2D screen. However, we did not observe significant differences in the accuracy of the counting task between visualization technologies in the elderly participants. Similarly, the preliminary results from the five brain-injured patients do not indicate any potential effect of the visualization technology on the cognitive load measured with the counting task. Although we expected the elderly and brain-injured populations to be more sensitive to a possible change in cognitive load – as old age is associated with cognitive decline [42] and patients might suffer from cognitive impairment [3] – our results are in line with our previous experiment with healthy young participants [23].

We observed that the counting task accuracy was relatively high in both elderly and brain-injured populations, indicating that the parallel cognitive task might have been too easy to elicit enough mistakes to see a difference across the visualization technologies. We reduced the difficulty of the cognitive task from our previous study with healthy young participants by reducing the number of total fruits (120 in the previous experiment, 102 with elderly participants, and 48 with brain-injured patients) and the maximum number of fruits in a block (24 in the previous experiment, 18 with elderly participants, and 12 with brain-injured patients) to adapt to the new populations. However, it seems that we ended up with a not challenging enough parallel cognitive task. The use of other cognitive tasks such as continuous monitoring – e.g., measuring the reaction time to a simple stimuli, such as a color change [43] –, sensory discrimination – e.g., measuring the reaction time to recognize a given stimuli, such as a specific haptic signal [44] –, or arithmetic operations – e.g.,

backwards counting [45] – might be more challenging. Furthermore, the non-continuous nature of the cognitive and motor tasks in our experiments might have lead to participants prioritizing the cognitive task over the motor task, resulting in a degradation of the movement quality metrics while the accuracy of the cognitive task remained high.

Regarding the self-reported cognitive load evaluated with the RTLX questionnaire, we found no significant difference across visualization technologies in the elderly participants, in line with our previous results with young healthy participants [24]. However, in the small group of brain-injured patients, the self-reported cognitive load appeared to be higher with the 2D screen than with AR, which also seemed higher than with IVR. This could potentially be due to the known cognitive impairments in brain-injured patients, who might have a different sensitivity to the potential cognitive load induced by the visuospatial transformation with the 2D screen. However, this observation must be further evaluated with a larger sample size of patients.

Importantly, we found significant differences across visualization technologies on the movement onset – i.e., the time lapsed between the appearance of the fruit and the start of the movement. Participants were asked to start to say aloud the counting value and the type of fruit before moving. Several studies have found an association between cognitive load and reaction times [44, 46]. We found that IVR significantly reduced the movement onset, compared to AR and 2D screen conditions in the elderly participants. Movements performed with AR also resulted in significantly shorter movement onset times than with the 2D screen. This difference was more obvious in movements that required moving towards fruit locations that involved the depth dimension. A similar trend was observed in brain-injured patients. Thus, performing reaching movements visualized on the 2D screen, especially those involving the depth dimension, might be associated with a higher cognitive load. However, we can not assume with certainty that longer movement onsets reflect higher cognitive load, as the onset was computed with a fixed velocity threshold. Thus, differences in pure motor aspects (i.e., the movement speed) might also lead to differences in movement onset. Yet, differences in the peak velocity between visualization technologies in the brain-injured patients were rather small, while the differences in the movement onset between these conditions were more obvious. Similarly, the differences in the peak velocity between the AR and 2D screen conditions were not significant in the elderly participants, while differences in the movement onset between these conditions reached significance.

The fact that participants could adapt their task performance strategy (i.e., take more time to count before

reaching) may have mitigated the subjectively experienced cognitive load and, therefore, differences in the questionnaires across conditions could not be observed. Other cognitive tasks requiring continuous attention may be more powerful in detecting changes in the cognitive load, such as counting (backwards), performing simple arithmetic's (for example, subtracting 7 starting from 100), citing the alphabet, etc.

To conclude, our results did not show differences between visualization technologies in the cognitive load, measured subjectively with the RTLX questionnaire and objectively with the cognitive counting task. However, we observed longer reaction times in the 2D screen condition, suggesting that the movement visualization on 2D screens might, indeed, increase the cognitive load. Importantly, the first self-reported assessments with brain-injured patients suggest a lower cognitive load when visualizing their movements with HMDs.

#### HMDs Do Not Significantly Impact Motivation

We expected that participants' motivation would be higher with HMDs than with the 2D screen, either indirectly due to the improved movement quality or directly due to the more naturalistic movement visualization [47, 24]. However, contrary to our expectations, we did not find differences in participants' motivation across visualization technologies. This result differs from the one reported in our previous experiment with young adults, where higher motivation was observed with IVR HMD compared to the 2D screen [24].

This could be interpreted as a potential reduction in the interest of elderly participants in new technologies. In our previous study, we recruited young adults from 19 to 42 years old. Other similar studies that found higher motivation when practicing with HMDs vs. 2D screens also included only young participants, e.g., in Born *et al.* participants were between 18 to 24 years old [48]. Similarly, in the study of Ijsselsteijn *et al.* [47], authors found that a higher immersion led to a higher motivation with a study population closer to our previous study (mean 41.3 y.o.). Thus, the high motivation associated with the use of HMDs might be age dependent. This difference highlights the importance of having studies with an age-matched population before drawing conclusions for clinical applications.

Nevertheless, it is important to note that, in the experiment with elderly participants, the recreated virtual environment was more complex than the one employed in our experiment with young participants, as it represented the real world with a higher fidelity. Being immersed in a simpler and less realistic virtual environment might potentially have increased the young

participants' motivation as they might have felt immersed in a virtual environment different than the real room. On the contrary, the realistic virtual environment employed with the elderly participants might have reduced their potential interest on IVR, as they were just immersed in a virtual environment that did not differ much from the real room.

#### HMDs Seem to Enhance Usability Only in Brain-injured Patients

We also expected the more naturalistic movement visualization offered by HMDs to increase the system usability. However, the differences in usability between visualization technologies were not significant in the elderly participants, while they remain rather high through all the conditions. This contrasts with the first results observed with brain-injured patients, who rated the 2D screen visualization as less usable than HMDs. However, the between-subject variability in the usability scores of the 2D screen is rather large compared to the IVR HMD. More patients are needed to confirm this difference, but our preliminary results seem to point out that HMDs are perceived as more usable than 2D screens by brain-injured patients.

Yet, it remains unclear why the elderly participants did not rate the IVR HMD as more usable than the 2D screen, as observed in the younger population [24] and brain-injured patients. A potential rationale might be that elderly participants are less familiar with new technologies than young adults. Differences between elderly participants and brain-injured patients could arise from differences in the complexity of the whole system – one of the aspects rated in the system usability questionnaire [34] – between experiments. With the elderly participants, the overall system had a relatively low complexity as they were only holding a virtual controller in the 2D screen condition. Having to wear an HMD might be a significant addition in complexity, compensating for the more naturalistic visualization. However, in the experiment with brain-injured patients, the entire system setup included the mechanical exoskeleton attached to their paretic arm. The addition of a wearable display might not have been perceived as a significant increase in the complexity of the entire system. This suggests that the combination of HMDs with rehabilitation devices is technically feasible and well accepted by the clinical population. Yet, this should be further studied with a larger population, including not only patients, but also therapists.

To conclude, our results suggest that the addition of new technologies such as HMDs has no negative impact on the system usability, as elderly participants reported equally high usability (> 80/100) compared to a conventional 2D screen. Moreover, our first insights gained in brain-injured patients suggest that the

clinical setting could especially benefit from the use of HMDs.

### Study Limitations & Future Research

The most limiting aspect of our study is the small sample size of neurologic patients that prevented us from running statistical analyses and draw conclusions over the measured data. Unfortunately, the current COVID pandemic limited the access to the clinics. Continuing this study with more brain-injured patients, once restrictions are lifted, is our future goal. Yet, we believe that the insights gained in this feasibility study are important to the rehabilitation community.

A second limitation of our study is how we measured cognitive load. The measurement with a dual-task paradigm is assumed to be a more direct and objective measurement technique than questionnaires [49]. However, the validity of our counting task as a dual task might be compromised, as participants might have prioritized the cognitive task over the motor task as suggested by the observed differences in the movement onset. To avoid relying on subjective reports and to have a more direct measurement of cognitive load, future research should integrate physiological measures of cognitive load previously shown to be reliable, such as skin conductance [50], eye movements [51], pupil dilatation [52, 53], as well as heart rate variability [54], and electroencephalography (EEG) [55].

Another limitation, which affects only the experiment with brain-injured patients, might be the potential visuohaptic conflict between the haptic stimuli – due to the weight support applied by the assistive device – and the visual absence of the device in the VE, i.e., the exoskeleton was not visible in the VE. Although it is unknown how this sensory conflict might have affected the patients in their movement quality or motivation and cognitive load reporting, recent evidence suggests that do not visualizing assistive devices during training in immersive VR does not affect the users' motivation, performance, nor visual attention, at least in a healthy young population [56].

### Conclusion

This study presents results from two experiments performed with twenty elderly participants and a small group of five subacute brain-injured patients to evaluate and compare the effect of different visualization technologies (an HTC Vive Pro for immersive VR, a Meta 2 for augmented reality, and a computer 2D screen) on movement quality, cognitive load, motivation, and usability.

The more naturalistic movement visualization and increased depth perception with head-mounted displays improved the quality of the 3D reaching movements, compared to a conventional computer 2D

screen. The HMDs might also have reduced the cognitive load, as measured by the time between stimulus presentation and movement onset. However, we did not find significant differences in subjective self-reports of cognitive load or in counting accuracy in the parallel counting task in the elderly healthy participants. Finally, although elderly and clinical populations might not be familiar with HMDs, participants rated them as highly usable, encouraging their usage in future VR-based rehabilitation interventions.

### Appendix

Text for this section. . .

#### Acknowledgements

The authors would like to thank Magdalena Eichenberger for her help with the recruitment of patients, Dr. Serena Maggioni from Hocoma for her support with the ArmeoSpring interfacing, Prof. Robert Riener for letting us borrow their Meta 2, Raphael Rätz for the 3D-printed fixation, and all the cleaning staff of the Anna-Seiler-Haus for their availability to open the doors in the late development evenings.

#### Funding

This work was supported in part by the Swiss National Science Foundation under Grant PP00P2 163800 and in part by the Swiss National Center of Competence in Research (NCCR Robotics).

#### Availability of data and materials

The dataset presented in this study can be found online in the following repository: [https://zenodo.org/record/6631771.YqV\\_H\\_XZBw2x](https://zenodo.org/record/6631771.YqV_H_XZBw2x).

#### Ethics approval and consent to participate

The study was approved by the local Ethics Committee (ref.: 2017-02,195) and conducted in compliance with the Declaration of Helsinki. All participants gave their written consent to participate in the study.

#### Competing interests

The authors declare that they have no competing interests.

#### Authors' contributions

NW contributed to the implementation of the virtual training environment, study design, experimental data acquisition, and data analysis. KAB contributed to the study design, experimental data acquisition, and data analysis. JP-A contributed to the implementation of the virtual training environment and study design. RMM contributed to the study design and recruitment of brain-injured patients. LM-C supervised the project and contributed to the study design and data analysis. All authors contributed to writing and revising the manuscript. All authors read and approved the final manuscript.

#### Authors' information

Motor Learning and Neurorehabilitation Laboratory, ARTORG Center for Biomedical Engineering Research, University of Bern, Freiburgstrasse 3, 3010, Bern, Switzerland

Nicolas Wenk, Karin A. Buetler Joaquin Penalver-Andres Laura Marchal-Crespo

Department of Neurology, University Neurorehabilitation, University Hospital Bern (Inselspital), University of Bern, Bern, Switzerland  
René M. Müri

Department of Cognitive Robotics, Delft University of Technology, Mekelweg 2, 2628 CD, Delft, the Netherlands

Laura Marchal-Crespo

#### Author details

<sup>1</sup>Motor Learning and Neurorehabilitation Laboratory, ARTORG Center for Biomedical Engineering Research, University of Bern, Bern, Switzerland.

<sup>2</sup>Gerontechnology & Rehabilitation, ARTORG Center for Biomedical Engineering Research, University of Bern, Bern, Switzerland. <sup>3</sup>Department of Neurology, University Neurorehabilitation, University Hospital Bern

(Inselspital), University of Bern, Bern, Switzerland. <sup>4</sup>Department of Cognitive Robotics, Delft University of Technology, Delft, Netherlands.

## References

- Feigin, V.L., Brainin, M., Norrving, B., Martins, S., Sacco, R.L., Hacke, W., Fisher, M., Pandian, J., Lindsay, P.: World Stroke Organization (WSO): Global Stroke Fact Sheet 2022. *International Journal of Stroke* **17**(1), 18–29 (2022). doi:10.1177/17474930211065917
- Aho, K., Harmsen, P., Hatano, S., Marquardsen, J., Smirnov, V.E., Strasser, T.: Cerebrovascular disease in the community: results of a who collaborative study. *Bulletin of the World Health Organization* **58**, 113–30 (1980)
- Patel, B., Birns, J.: Post-Stroke Cognitive Impairment. In: *Manag. Post-Stroke Complicat.*, pp. 277–306. Springer, Cham (2015). doi:10.1007/978-3-319-17855-4\_12. [http://link.springer.com/10.1007/978-3-319-17855-4\\_12](http://link.springer.com/10.1007/978-3-319-17855-4_12)
- Kwakkel, G., Kollen, B., Lindeman, E.: Understanding the pattern of functional recovery after stroke: Facts and theories. *Restorative Neurology and Neuroscience* **22**, 281–299 (2004). doi:10.3233/RNN-130332
- Winters, C., van Wegen, E.E.H., Daffertshofer, A., Kwakkel, G.: Generalizability of the proportional recovery model for the upper extremity after an ischemic stroke. *Neurorehabilitation and Neural Repair* **29**, 614–622 (2015). doi:10.1177/1545968314562115
- Levac, D.E., Huber, M.E., Sternad, D.: Learning and transfer of complex motor skills in virtual reality: a perspective review. *Journal of NeuroEngineering and Rehabilitation* **16**, 121 (2019). doi:10.1186/s12984-019-0587-8
- Krakauer, J.W.: Motor learning: its relevance to stroke recovery and neurorehabilitation. *Current Opinion in Neurology* **19**, 84–90 (2006). doi:10.1097/01.wco.0000200544.29915.cc
- Kwakkel, G., van Peppen, R.V., Wagenaar, R.C., Dauphinee, S.W., Richards, C., Ashburn, A., Miller, K., Lincoln, N., Partridge, C., Wellwood, I., Langhorne, P.: Effects of augmented exercise therapy time after stroke: a meta-analysis. *Stroke* **35**, 2529–39 (2004). doi:10.1161/01.STR.0000143153.76460.7d
- Bayona, N.A., Bitensky, J., Salter, K., Teasell, R.: The role of task-specific training in rehabilitation therapies. *Topics in Stroke Rehabilitation* **12**, 58–65 (2005). doi:10.1310/BQM5-6YGB-MVJ5-WVCR
- Mulder, T., Hochstenbach, J.: Adaptability and flexibility of the human motor system: Implications for neurological rehabilitation. *Neural Plasticity* **8**, 131–140 (2001). doi:10.1155/NP.2001.131
- Kleim, J.A.: Synaptic Mechanisms of Learning, pp. 731–734. Elsevier, ??? (2009). doi:10.1016/B978-008045046-9.01316-4. <https://linkinghub.elsevier.com/retrieve/pii/B9780080450469013164>
- Maclean, N., Pound, P.: A critical review of the concept of patient motivation in the literature on physical rehabilitation. *Social science & medicine* (1982) **50**(4), 495–506 (2000). doi:10.1016/S0277-9536(99)00334-2
- Maclean, N., Pound, P., Wolfe, C., A, R.: Qualitative analysis of stroke patients' motivation for rehabilitation. *BMJ (Clinical research ed.)* **321**(7268), 1051–1054 (2000). doi:10.1136/bmj.321.7268.1051
- Putrino, D., Zanders, H., Hamilton, T., Rykman, A., Lee, P., Edwards, D.J.: Patient Engagement Is Related to Impairment Reduction During Digital Game-Based Therapy in Stroke. *Games Health J.* **6**(5), 295–302 (2017). doi:10.1089/g4h.2016.0108
- Wulf, G., Lewthwaite, R.: Optimizing performance through intrinsic motivation and attention for learning: The optimal theory of motor learning. *Psychonomic Bulletin & Review* **23**, 1382–1414 (2016). doi:10.3758/s13423-015-0999-9
- Mekbib, D.B., Han, J., Zhang, L., Fang, S., Jiang, H., Zhu, J., Roe, A.W., Xu, D.: Virtual reality therapy for upper limb rehabilitation in patients with stroke: a meta-analysis of randomized clinical trials. *Brain Inj.* **34**(4), 456–465 (2020). doi:10.1080/02699052.2020.1725126
- Rizzo, J.-R., Hosseini, M., Wong, E.A., Mackey, W.E., Fung, J.K., Ahdoot, E., Rucker, J.C., Raghavan, P., Landy, M.S., Hudson, T.E.: The Intersection between Ocular and Manual Motor Control: Eye–Hand Coordination in Acquired Brain Injury. *Front. Neurol.* **8**(JUN) (2017). doi:10.3389/fneur.2017.00227
- Mousavi Hondori, H., Khademi, M., Dodakian, L., McKenzie, A., Lopes, C.V., Cramer, S.C.: Choice of Human–Computer Interaction Mode in Stroke Rehabilitation. *Neurorehabil. Neural Repair* **30**(3), 258–265 (2016). doi:10.1177/1545968315593805
- Liebermann, D.G., Berman, S., Weiss, P.L., Levin, M.F.: Kinematics of reaching movements in a 2-d virtual environment in adults with and without stroke. *IEEE Trans. Neural Syst. Rehab. Eng.* **20**(6), 778–787 (2012). doi:10.1109/TNSRE.2012.2206117
- Schweighofer, N., Wang, C., Mottet, D., Laffont, I., Bakthi, K., Reinkensmeyer, D.J., Rémy-néris, O.: Dissociating motor learning from recovery in exoskeleton training post-stroke. *Journal of NeuroEngineering and Rehabilitation* **15**, 89 (2018). doi:10.1186/s12984-018-0428-1
- Levin, M.F., Snir, O., Liebermann, D.G., Weingarden, H., Weiss, P.L.: Virtual reality versus conventional treatment of reaching ability in chronic stroke: Clinical feasibility study. *Neurology and Therapy* **1**, 3 (2012). doi:10.1007/s40120-012-0003-9
- Knaut, L.A., Subramanian, S.K., McFadyen, B.J., Bourbonnais, D., Levin, M.F.: Kinematics of pointing movements made in a virtual versus a physical 3-dimensional environment in healthy and stroke subjects. *Archives of Physical Medicine and Rehabilitation* **90**, 793–802 (2009). doi:10.1016/j.apmr.2008.10.030
- Wenk, N., Penalver-Andres, J., Palma, R., Buetler, K.A., Muri, R., Nef, T., Marchal-Crespo, L.: Reaching in Several Realities: Motor and Cognitive Benefits of Different Visualization Technologies. In: *2019 IEEE 16th Int. Conf. Rehabil. Robot.*, pp. 1037–1042. IEEE, Toronto, Canada (2019). doi:10.1109/ICORR.2019.8779366
- Wenk, N., Penalver-Andres, J., Buetler, K.A., Nef, T., Müri, R.M., Marchal-Crespo, L.: Effect of Immersive Visualization Technologies on Cognitive Load, Motivation, Usability, and Embodiment. *Virtual Real.* (2021). doi:10.1007/s10055-021-00565-8
- Gerig, N., Mayo, J., Baur, K., Wittmann, F., Riener, R., Wolf, P.: Missing depth cues in virtual reality limit performance and quality of three dimensional reaching movements. *PLOS ONE* **13**(1), 1–18 (2018). doi:10.1371/journal.pone.0189275
- Palacios-Navarro, G., Hogan, N.: Head-Mounted Display-Based Therapies for Adults Post-Stroke: A Systematic Review and Meta-Analysis. *Sensors* **21**(4), 1111 (2021). doi:10.3390/s21041111
- Laver, K., Lange, B., George, S., Deutsch, J., Saposnik, G., Crotty, M.: Virtual reality for stroke rehabilitation (Review). *Cochrane Database Syst Rev* (11) (2017). doi:10.1002/14651858.CD008349.pub4
- Cabeza, R.: Cognitive neuroscience of aging: Contributions of functional neuroimaging. *Scandinavian Journal of Psychology* **42**(3), 277–286 (2001). doi:10.1111/1467-9450.00237. <https://onlinelibrary.wiley.com/doi/pdf/10.1111/1467-9450.00237>
- Park, D.C., Reuter-Lorenz, P.: The adaptive brain: Aging and neurocognitive scaffolding. *Annual Review of Psychology* **60**(1), 173–196 (2009). doi:10.1146/annurev.psych.59.103006.093656. <https://doi.org/10.1146/annurev.psych.59.103006.093656>
- Fagard, J., Chapelain, A., Bonnet, P.: How should “ambidexterity” be estimated? Laterality Asymmetries Body, *Brain Cogn.* **20**(5), 543–570 (2015). doi:10.1080/1357650X.2015.1009089
- Oldfield, R.C.: The assessment and analysis of handedness: The Edinburgh inventory. *Neuropsychologia* **9**(1), 97–113 (1971). doi:10.1016/0028-3932(71)90067-4
- Hart, S.G.: NASA-TLX: 20 Years Later. *Proc. Hum. Factors Ergon. Soc. Annu. Meet.*, 904–908 (2006). doi:10.1177/154193120605000909
- Reynolds, L.: Measuring Intrinsic Motivations. In: *Handb. Res. Electron. Surv. Meas.*, pp. 170–173. IGI Global, ??? (2007). doi:10.4018/978-1-59140-792-8.ch018
- Brooke, J.: SUS: A “quick and dirty” usability scale. In: Jordan, P.W., Thomas, B., Weerdmeester, B.A., McClelland, I.L. (eds.) *Usability Eval. Ind.*, pp. 189–194. Taylor & Francis, London (1996). [https://cui.unige.ch/isi/icle-wiki/\\_media/ipm:test-suschart.pdf](https://cui.unige.ch/isi/icle-wiki/_media/ipm:test-suschart.pdf)
- Harris, P.A., Taylor, R., Thielke, R., Payne, J., Gonzalez, N., Conde, J.G.: Research electronic data capture (REDCap) - a metadata-driven methodology and workflow process for providing translational research informatics support. *J Biomed Inform* (2009). doi:10.1016/j.jbi.2008.08.010
- Lambercy, O., Lünenburger, L., Gassert, R., Bolliger, M.: In: Dietz, V., Nef, T., Rymer, W.Z. (eds.) *Robots for Measurement/Clinical Assessment*, pp. 443–456. Springer, London (2012)
- Viau, A., Feldman, A.G., McFadyen, B.J., Levin, M.F.: Reaching in

- reality and virtual reality: A comparison of movement kinematics in healthy subjects and in adults with hemiparesis. *Journal of NeuroEngineering and Rehabilitation* **1** (2004). doi:10.1186/1743-0003-1-11
38. Kim, W.-S., Cho, S., Ku, J., Kim, Y., Lee, K., Hwang, H.-J., Paik, N.-J.: Clinical application of virtual reality for upper limb motor rehabilitation in stroke: Review of technologies and clinical evidence. *Journal of Clinical Medicine* **9**, 3369 (2020). doi:10.3390/jcm9103369
  39. Huang, V.S., Krakauer, J.W.: Robotic neurorehabilitation: a computational motor learning perspective. *Journal of NeuroEngineering and Rehabilitation* **6**, 5 (2009). doi:10.1186/1743-0003-6-5
  40. Nordin, N., Xie, S.Q., Wünsche, B.: Assessment of movement quality in robot- assisted upper limb rehabilitation after stroke: a review. *Journal of NeuroEngineering and Rehabilitation* **11**, 137 (2014). doi:10.1186/1743-0003-11-137
  41. Kwakkel, G., van Wegen, E.E.H., Burridge, J.H., Winstein, C.J., van Dokkum, L.E.H., Murphy, M.A., Levin, M.F., Krakauer, J.W.: Standardized measurement of quality of upper limb movement after stroke: Consensus-based core recommendations from the second stroke recovery and rehabilitation roundtable. *Neurorehabilitation and Neural Repair* **33**(11), 951–958 (2019). doi:10.1177/1545968319886477. <https://doi.org/10.1177/1545968319886477>
  42. Park, D.C., Schwarz, N.: *Cognitive Aging: A Primer*. Psychology Press, ??? (2008). <https://books.google.ch/books?id=z5rlkQEACAAJ>
  43. Leppink, J., Paas, F., der Vleuten, C.P.M.V., Gog, T.V., Merriënboer, J.J.G.V.: Development of an instrument for measuring different types of cognitive load. *Behavior research methods* **45**, 1058–72 (2013). doi:10.3758/s13428-013-0334-1
  44. Rojas, D., Haji, F., Shewaga, R., Kapralos, B., Dubrowski, A.: The impact of secondary-task type on the sensitivity of reaction-time based measurement of cognitive load for novices learning surgical skills using simulation. *Studies in health technology and informatics* **196**, 353–9 (2014). doi:10.3233/978-1-61499-375-9-353
  45. Ocampo, R., Tavakoli, M.: Visual-haptic colocation in robotic rehabilitation exercises using a 2d augmented-reality display, pp. 1–7. *IEEE, ???* (2019). doi:10.1109/ISMR.2019.8710185. <https://ieeexplore.ieee.org/document/8710185/>
  46. van Winsum, W.: The effects of cognitive and visual workload on peripheral detection in the detection response task. *Human Factors: The Journal of the Human Factors and Ergonomics Society* **60**, 855–869 (2018). doi:10.1177/0018720818776880
  47. IJsselstein, W.A., Kort, Y.A.W.d., Westerink, J., Jager, M.d., Bonants, R.: *Virtual Fitness: Stimulating Exercise Behavior through Media Technology*. Presence: Teleoperators and Virtual Environments **15**(6), 688–698 (2006). doi:10.1162/pres.15.6.688. <https://direct.mit.edu/pvar/article-pdf/15/6/688/1624847/pres.15.6.688.pdf>
  48. Born, F., Abramowski, S., Masuch, M.: Exergaming in vr: The impact of immersive embodiment on motivation, performance, and perceived exertion. 2019 11th International Conference on Virtual Worlds and Games for Serious Applications, VS-Games 2019 - Proceedings, 1 (2019). doi:10.1109/VS-Games.2019.8864579
  49. Brünken, R., Plass, J.L., Leutner, D.: Direct measurement of cognitive load in multimedia learning. *Educational Psychologist* **38**(1), 53–61 (2003). doi:10.1207/S15326985EP3801\_7. [https://doi.org/10.1207/S15326985EP3801\\_7](https://doi.org/10.1207/S15326985EP3801_7)
  50. Naccache, L., Dehaene, S., Cohen, L., Habert, M.-O., Guichart-Gomez, E., Galanaud, D., Willer, J.-C.: Effortless control: executive attention and conscious feeling of mental effort are dissociable. *Neuropsychologia* **43**, 1318–1328 (2005). doi:10.1016/j.neuropsychologia.2004.11.024
  51. Eckstein, M.K., Guerra-Carrillo, B., Singley, A.T.M., Bunge, S.A.: Beyond eye gaze: What else can eyetracking reveal about cognition and cognitive development? *Developmental Cognitive Neuroscience* **25**, 69–91 (2017). doi:10.1016/j.dcn.2016.11.001
  52. van der Wel, P., van Steenbergen, H.: Pupil dilation as an index of effort in cognitive control tasks: A review. *Psychonomic Bulletin & Review* **25**, 2005–2015 (2018). doi:10.3758/s13423-018-1432-y
  53. Marquart, G., de Winter, J.: Workload assessment for mental arithmetic tasks using the task-evoked pupillary response. *PeerJ Computer Science* **1**, 16 (2015). doi:10.7717/peerj-cs.16
  54. Solhjo, S., Haigney, M.C., McBee, E., van Merriënboer, J.J.G., Schuwirth, L., Artino, A.R., Battista, A., Ratcliffe, T.A., Lee, H.D., Durning, S.J.: Heart rate and heart rate variability correlate with clinical reasoning performance and self-reported measures of cognitive load. *Scientific Reports* **9**, 14668 (2019). doi:10.1038/s41598-019-50280-3
  55. Skulmowski, A., Rey, G.D.: Measuring cognitive load in embodied learning settings. *Frontiers in Psychology* **8**, 1191 (2017). doi:10.3389/fpsyg.2017.01191
  56. Wenk, N., Jordi, M.V., Buetler, K.A., Marchal-Crespo, L.: Hiding assistive robots during training in immersive vr does not affect users' motivation, presence, embodiment, performance, nor visual attention. *IEEE Transactions on Neural Systems and Rehabilitation Engineering* **30**, 390–399 (2022). doi:10.1109/TNSRE.2022.3147260

## Figures

## Tables

## Additional Files

Additional file 1 — Sample additional file title

Additional file descriptions text (including details of how to view the file, if it is in a non-standard format or the file extension). This might refer to a multi-page table or a figure.

Additional file 2 — Sample additional file title

Additional file descriptions text.