

Proof of Concept of a Multimodal Intravital Molecular Imaging System for Tumour Transpathology Investigation

Zhen Liu

Technical University of Munich: Technische Universität München

Tao Cheng

Technical University of Munich: Technische Universität München

Stephan Düwel

Technical University of Munich: Technische Universität München

Ziying Jian

Technical University of Munich: Technische Universität München

Geoffrey J. Topping

Technical University of Munich: Technische Universität München

Katja Steiger

Technical University of Munich: Technische Universität München

Qian Wang

Technical University of Munich: Technische Universität München

Rickmer Braren

Technical University of Munich: Technische Universität München

Sybille Reder

Technical University of Munich: Technische Universität München

Markus Mittelhäuser

Technical University of Munich: Technische Universität München

Christian Hundshammer

Technical University of Munich: Technische Universität München

Benedikt Feuerecker

Technical University of Munich: Technische Universität München

Sung-Cheng Huang

University of California Los Angeles

Markus Schwaiger

Technical University of Munich: Technische Universität München

Franz Schilling

Technical University of Munich: Technische Universität München

Sibylle Ziegler

Technical University of Munich: Technische Universität München

Kuangyu Shi (✉ kuangyu.shi@dbmr.unibe.ch)

Universität Bern <https://orcid.org/0000-0002-8714-3084>

Research Article

Keywords: Transpathology, Intravital imaging, Multimodal imaging, Window chamber, Tumour microenvironment, Positron imaging, MRI, Fluorescence microscopy

Posted Date: May 20th, 2021

DOI: <https://doi.org/10.21203/rs.3.rs-526621/v1>

License: © ⓘ This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

Version of Record: A version of this preprint was published at European Journal of Nuclear Medicine and Molecular Imaging on October 15th, 2021. See the published version at <https://doi.org/10.1007/s00259-021-05574-y>.

Proof of concept of a multimodal intravital molecular imaging system for tumour transpathology investigation

Authors: Zhen Liu^{1,2}, Tao Cheng¹, Stephan Düwel¹, Ziyang Jian¹, Geoffrey J. Topping¹, Katja Steiger³, Qian Wang¹, Rickmer Braren⁴, Sybille Reder¹, Markus Mittelhäuser¹, Christian Hundshammer¹, Benedikt Feuerecker¹, Sung-Cheng Huang⁵, Markus Schwaiger¹, Franz Schilling¹, Sibylle I. Ziegler^{1,6}, Kuangyu Shi^{1,7,8}

Author information

¹ Department of Nuclear Medicine, School of Medicine, Technische Universität München, Munich, Germany

² Qingdao Cancer Institute, The Affiliated Hospital of Qingdao University, Qingdao University, Qingdao, China

³ Department of Pathology, School of Medicine, Technische Universität München, Munich, Germany

⁴ Department of Radiology, Technische Universität München, Munich, Germany

⁵ Department of Molecular and Medical Pharmacology, David Geffen School of Medicine, University of California, Los Angeles, USA

⁶ Department of Nuclear Medicine, University Hospital LMU Munich, Germany

⁷ Department of Nuclear Medicine, University of Bern, Switzerland

⁸ Department of Informatics, Technische Universität München, Munich, Germany

***Corresponding author:**

Prof. Kuangyu Shi

Dept. Informatics

Technical University of Munich

Email: k.shi@tum.de

Abstract

Background: Transpathology highlights the interpretation of underlying physiology behind molecular imaging. However, it remains challenging due to the discrepancies between *in vivo* and *in vitro* measurements and difficulties of precise co-registration between multi-scaled images. This study aims to develop a multimodal intravital molecular imaging (MIMI) system as a tool for *in vivo* tumour transpathology investigation.

Methods: The proposed MIMI system integrates high-resolution positron imaging, magnetic resonance imaging (MRI) and microscopic imaging on a dorsal skin window chamber on a nude rat. The window chamber frame was designed to be compatible with multimodal imaging and its fiducial markers were customized for precise physical alignment among modalities. The co-registration accuracy was evaluated based on phantoms with thin catheters. For proof of concept, the human colorectal adenocarcinoma cell line HT-29 was imaged. The tissue within the window chamber was sectioned, fixed, hematoxylin-eosin (HE) stained for comparison with multimodal *in vivo* imaging.

Results: With the physical alignment via fiducial markers, the co-registration errors of the MIMI system were 0.18 ± 0.27 mm between MRI and positron imaging, 0.19 ± 0.22 mm between positron imaging and microscopic imaging, and 0.15 ± 0.27 mm between MRI and microscopic imaging. A pilot test demonstrated that the MIMI system provides an integrative visualization of the tumour anatomy, perfusion and metabolism of the *in vivo* tumour microenvironment.

Conclusions: The established MIMI system provided a co-registered *in vivo* platform for trans-scale and transparent investigation of the underlying pathology behind imaging, which has the potential to enhance the translation of molecular imaging.

Keywords: Transpathology; Intravital imaging; Multimodal imaging; Window chamber; Tumour microenvironment; Positron imaging; MRI; Fluorescence microscopy

Background

Transpathology is a new concept to summarize the endeavor of molecular imaging for deciphering underlying pathophysiology [1, 2], which consists of trans-scale, transparent and translational investigation of imaging signals (Fig. 1A). However, the practice of transpathology is complicated by discrepancies between *in vivo* imaging and *ex vivo* pathology. Conventionally, tissues need to be sampled or resected for the investigation by microscopy [3-6]. Although these *in vitro* methods have been widely used in various applications, they are destructive and have limited ability to provide insight into *in vivo* dynamics [7]. Another crucial problem for the comparison between imaging and pathology is the co-registration of *in vivo* and *ex vivo* measurements. It is difficult to find useful landmarks or similarities between the images with such a huge resolution difference and typical co-registration algorithms are not applicable [8]. Also, the complicated preparation procedure of the histology sections introduces substantial distortions, and it is thus almost impossible to localize the physiological features precisely in conventional imaging methods.

Intravital imaging is a powerful tissue investigation method to provide high-resolution information of the tissue microenvironment in an intact animal [9, 10]. Different transparent window models have been developed to investigate various types of tumours. Chronic window models such as dorsal skin windows and cranial windows expose a stable tumour microenvironment and allow longitudinal observation of tumour evolution [11, 12]. Intravital imaging can identify *in vivo* tissue morphological and metabolic characteristics like pH or pO_2 , using various investigation methods such as fluorescence microscopy [13-15] and phosphorescence lifetime imaging [16, 17]. The integration of clinical imaging such as MRI or PET with intravital imaging facilitates identification of detailed physiological features of imaging elements directly from the same intact tissue [18, 19]. In the study, a dedicated surface receiver coil was applied to obtain high quality MRI [18]. With careful design of the dynamic protocol, DCE MRI was acquired to quantify the perfusion (blood supply time) of the tissue [18]. In another study, direct positron imaging was proposed to improve the sensitivity and resolution of PET imaging within a window chamber [19].

The aim of this study is to establish a multimodal intravital molecular imaging (MIMI) system to support the investigation of transpathology (Fig. 1B). It is based on animal model with a dorsal skin window chamber, which is compatible with the high-resolution MRI, positron imaging and microscopic imaging and which allows precise co-registrations. A pilot test of the multi-modal trans-scale imaging and the co-registration accuracy was performed.

Materials and methods

Dorsal skin window chamber for multimodal intravital imaging

For transpathology research, a MIMI system is proposed to integrate positron imaging, MRI and optical imaging (e.g., microscope) within an intact and rigid frame (Fig. 1B). This rigid frame is established using a dorsal skin window chamber, which is compatible with the above-mentioned imaging modalities, including fiducial markers for positioning and localization. The chamber is made from polyetheretherketone (PEEK), which is rigid but flexible, and is chemically inert to majority organic and inorganic chemicals and solvents [18]. The mounting pins can be used to fix a positron camera accurately within the chamber. The fixation screw threads and suture holes provide additional fiducial markers for localization with imaging such as MRI, fluorescence imaging, and positron imaging.

Window chamber implantation and tumour transplantation

Athymic RNU nude rats (CrI: NIH-Foxn1^{rnu}, Charles River) were employed for the *in vivo* test of the MIMI system. The implantation of the multimodal compatible dorsal skin window chamber onto the RNU rat followed the literature [20, 21] with some adaptations. During the chamber implantation, rats were anesthetized with inhalation of isoflurane (2% in oxygen, 2 L/min). A single-cell suspension of the human colorectal adenocarcinoma cell line HT29 (2×10^6 cells in 0.05 ml PBS) was prepared for subcutaneous injection onto the fascia side of the intact skin layer within the window area. All animal studies were approved by the local government committee for animal protection and welfare (Tierschutzbehörde, Regierung von Oberbayern, with license protocol number 18-13).

Positron imaging

A positron camera with a physical resolution of 230 μm was employed for high-resolution 2D imaging within the window chamber area [22, 23]. The window chamber with intact skin was fixed to an adapter (Supplemental Fig. 2) and then mounted to the positron camera via the above-mentioned mounting pins. A Mylar sheet (6 μm) was placed on the surface of the camera to prevent possible contact with tissue fluid. Positron imaging of 10 minutes was acquired at 50 min post injection of ca.150 kBq/g body weight of [^{18}F]FDG under anesthesia.

MR imaging

The MR images were scanned with a 7T preclinical MRI system (Discovery MR901, Agilent Technologies, Santa Clara, USA). The rat was fixed on the MR bed with air heating during anesthesia and monitoring of the electrocardiogram heart rate, breathing rate, and body temperature with pressure sensitive sensing pad (RAPID Biomedical GmbH). A single-channel flexible receiver coil (diameter 30 mm, RAPID Biomedical GmbH) was placed on top of the window chamber. A quadrature birdcage resonator (72 mm inner diameter, RAPID Biomedical GmbH) was used for radio frequency (RF) transmission. T1 weighted images using fast spin echo sequence (TR=300 ms, TE=1 ms, 192×192 matrix, 1 mm slice thickness, $4 \text{ cm} \times 4 \text{ cm}$ FOV, number of excitations (NEX) = 4. Flip angle 60°), T2 weighted images (TR=3000 ms, TE=35 ms, 192×192 matrix, 1 mm slice thickness, $4 \text{ cm} \times 4 \text{ cm}$ FOV, NEX =4, Flip angle 60°) were acquired after positioning. Dynamic contrast enhanced (DCE) MRI was acquired during the injection of Gd-DTPA solution (0.25 mmol/kg) with a flow rate of 160 ml/h using a syringe pump (Pump Elite 11, Harvard Apparatus, Cambridge, USA). The DCE MRI was acquired using the TRICKS sequence (time resolved imaging of contrast kinetics) [24]. TRICKS acquisition was started 15s before the start of the pump injection. The parameters were: TR = 4 ms, TE = 1.7 ms, 192×192 matrix, 1 mm slice thickness, $4 \text{ cm} \times 4 \text{ cm}$ FOV, Flip angle: 40° . Fifty-six phases were obtained with 28 images in each phase. Each phase measured with a

temporal resolution of 3 seconds. After the DCE-MRI, another T1-weighted MRI scan was acquired with the same the parameters as before the contrast agent injection.

Optical imaging

Pathophysiological information was observed with a fluorescence microscope (Imager. M2, Zeiss, Germany) equipped with a black/white charge-coupled device (CCD) camera (AxioCam MRm). Fluorescein isothiocyanate (FITC)-dextran (Sigma Aldrich, St. Louis, MO, USA) was administrated to measure perfusion under MMF (Midazolam/medetomidine/fentanyl with a concentration in mg/ml of 5/1/0.05) anesthesia. The window chamber was fixed onto the adapter (Supplemental Fig. 2) and then fixed to the fluorescence microscope. A transparent coordinate plate (Supplemental Fig. 3) was mounted onto the window chamber for localization. A fluorescence image of 1.25× magnification with a green fluorescent protein (GFP) filter was recorded.

Phantom test

To assess the co-registration accuracy for different imaging modalities, phantoms were prepared with two or three thin catheters (I.D.: 0.3 mm, O.D.: 0.6 mm) fixed independently within the window chamber using glue and transparent tape. Phantoms were imaged with positron imaging, MRI and fluorescence microscopy. The catheters were filled with [¹⁸F]FDG (1 MBq/ml) for positron imaging, saline during T1 weighted MRI imaging and fluorescein isothiocyanate–dextran (FITC)-dextran during fluorescence imaging.

Ex vivo histological staining

After imaging, the rat was euthanized by administration of 0.5 ml pentobarbital sodium via tail vein injection during the anesthesia state (Narcoren, 16 g/100 ml, Merial GmbH, Germany). The skin along the window area was cut and fixed with 4% para-formalin solution for 1 day, then sunk into 70% ethanol for 2 days. The fixed tissue block was embedded in paraffin and cut for hematoxylin-eosin (H&E) staining. The whole stained tissue slide was recorded by transmission light using a fluorescence microscopy (BZ-9000,

KEYENCE). Due to the limited FOV of the microscopy, the tissue within the window area cannot be covered within one microscopic image. Therefore, the tissue slide was recorded one by one using a 4-fold objective lens. The images were further combined into a new image with a larger FOV.

Data processing

All the primary data from different imaging modalities were aligned via the fiducial markers using PMOD (PMOD technologies Ltd, Zürich, Switzerland). For phantom measurements, the skeletons of the catheters were extracted by estimating the ridge lines of the imaging signals of the catheters with Gaussian function as medial function [25]. The errors of the co-registrations (i.e., the distances between the skeleton lines obtained from the corresponding imaging modalities) were estimated by comparing the skeleton lines.

Results

Accuracy of image co-registration from phantom test

Images from MRI, positron imaging, and fluorescence imaging were aligned via the fiducial markers. Example phantom images are displayed in Fig. 2, with skeleton lines of different modalities extracted from each phantom-tube are presented on the MRI image. The registration errors between three imaging modalities are plotted in Fig. 3, with statistics for 7 skeleton lines (from three phantoms and the corresponding multimodal imaging experiments) presented in each comparison plot. The co-registration errors were 0.18 ± 0.27 mm between MRI and positron imaging, 0.19 ± 0.22 mm between positron imaging and microscopic imaging, and 0.15 ± 0.27 mm between MRI and microscopic imaging.

Integrated tumour microenvironment imaging

Example results of multimodal imaging of a rat with the window chamber is depicted in Fig. 4. The tumour ($6.1 \text{ mm} \times 4.9 \text{ mm}$ in length and width) in the pre-contrast injection T1 weighted image was brighter compared with the surrounding tissue (Fig. 4A), and darker in the T2 weighted image (Fig. 4B). The T1 weighted MRI image after Gd-DTPA injection depicted the enhanced contrast of the tissue within the

window chamber (Fig. 4C). The border of the tumour was clearer after the contrast agent injection. The K^{trans} map of the MR image denoting the blood flow and vascular permeability (influx rate for the contrast agent into the extravascular extracellular space tissue from blood) is presented in Fig. 4D. A fluorescence image (FITC-dextran, Fig. 4E) of the window chamber visualizes the blood perfusion around the tumour tissue. The FITC-dextran fluorescence image of a smaller FOV inside the tumour showed a detailed blood vessel network in the micrometer resolution range. The complexity of the tumour vascular network shown in the fluorescence image was consistent with the MRI observation. From the positron imaging (Fig. 4F), the tumour had generally positive [^{18}F]FDG uptake. From the H&E staining image (Fig. 4G), two tumour parts were visualized. A small part of the tumour, indicated with blue circle in Fig. 4G was negative in positron imaging.

These three imaging modalities have trans-scaled imaging resolution. The spatial resolution of the MRI, fluorescence image, and positron imaging was 156 μm (pixel size), 5.16 μm , and 230 μm , respectively. The precise co-registration among these images was accomplished with the aid of the transparent plastic plate with reference pattern (refer to supplemental Fig. 3). Both the fluorescence and positron images can be precisely localized within the MRI image with the aid of the fiducial markers on the window chamber (red box in Fig. 4B). The location of the positron image is always fixed with reference to the four fixation pins, as the positron camera was mounted onto the window chamber with four holes around its detector.

Discussions

Co-registration between in vivo and ex vivo imaging

Pathology is considered as the gold standard for disease diagnosis. However, it is a sampling and test process, facing several limitations, such as invasiveness, incomprehensiveness due to biopsy sampling sites and sampling time, and missing *in vivo* changes due to limited sampling times. Imaging is a non-invasive tool for intravital observation of pathological changes. The concept of transpathology to linking the imaging with pathology facing two major obstacles for precise evaluation: 1) The discrepancies of scale and resolution between *in vivo* imaging and *ex vivo* pathology; and 2) The precise co-registration among various

trans-scaled imaging modalities and *ex vivo* pathology. Puri et al. proposed a method for accurate registration of PET images and histopathology slices [8]. They used sea urchin spines as fiducial markers for pathology and *ex vivo* CT imaging to localize the histopathology slices. The registration error between histopathology and *ex vivo* CT was reported of 0.86 ± 0.41 mm. The *ex vivo* CT images were then aligned to the *in vivo* PET images and the overall registration error between PET and histopathology was 3.0 ± 0.7 mm. In contrast to the registration via *ex vivo* anatomical imaging, the MIMI system employs the window chamber and assisting holders to immobilize the tissues during the imaging of different modalities. Fiducial markers were designed for the physical localization of the positron imaging and MRI. The localization of microscopic imaging is more difficult due to large difference in field of view (FOV) and resolution. A transparent plastic reference mounted to the fiducial markers with oriented coordination assists the alignment of the microscopic images. The microscopic imaging is very sensitive to tilting of the object. The special holder of the window chamber during microscopic imaging ensured the window chamber to be placed parallel to the microscopy's lens to avoid imaging blurring. These special designs of the MIMI system led to much smaller co-registration errors of 0.18 ± 0.27 mm between MRI and positron imaging, 0.19 ± 0.22 mm between positron imaging and microscopic imaging, and 0.15 ± 0.27 mm between MRI and microscopic imaging. The immobilized imaging and the fiducial coordination of the MIMI system facilitate accurate trans-scale image co-registration.

Multimodal molecular imaging

The combination of PET and MRI provides multimodal clinical or preclinical imaging to visualize anatomical, functional and metabolic features to support the optimization of diagnosis and therapy [26-29]. However, the increased complexity of overlapping or contradictory signal between different modalities within the same tumor due to intratumoral heterogeneity poses substantial challenges on investigation of underlying physiology [30, 31]. The integration of PET, MRI and intravital imaging in the MIMI system allows fingerprinting the physiological heterogeneity behind multimodal imaging for the same intact tissue [19, 32] and is therefore complementary to conventional preclinical PET/MR in the investigation. The quasi

2D imaging on intravital window allows higher resolution than conventional 3D PET or MR imaging. With surface coils it is possible to focus on the thin skin tissue for imaging with a relatively high sensitivity and resolution ($< 200 \mu\text{m}$) [32]. For the imaging of PET tracer, conventional 3D preclinical is not optimal for imaging of thin tissue within the observation window due to low intrinsic resolution and partial volume effects (PVE) [33]. The positron camera has intrinsically higher resolution of $230 \mu\text{m}$ for 2D imaging [22, 23], which is better than intrinsic resolution of typical 3D preclinical PET scanners [34]. In practice, positron imaging is not perfect 2D imaging either and measures the superposed signals from tissues close to the contacting surface. The positron imaging has only spill-in from tissues below the surface, while conventional 3D preclinical PET can have both spill-out and spill-in to the imaging surface. The sensitivity of positron camera is depth-dependent. The spill-in decreases as the depth increases with half at a depth of $235 \mu\text{m}$ and vanishes at a depth of $470 \mu\text{m}$ [35]. In contrast, the spill-in for a high-resolution 3D preclinical PET with 1 mm intrinsic resolution can be 80% from tissue at a depth of $235 \mu\text{m}$ and 50% at a depth of $470 \mu\text{m}$ according to theoretical estimation [36, 37]. Therefore, the proposed positron imaging is more appropriate for quasi-2D imaging of window chamber.

Limitations of the MIMI system

The proposed MIMI system has some limitations. (1) Although the fiducial marker facilitated accuracy co-registration for the 2D area within the observation window, it cannot help localize the depth of the microscopic image precisely (the Z-axis that perpendicular to the 2D window area). (2) The current study did proof-of-concept of the multimodal intravital imaging system, no in-depth physiological investigation has been performed. For the partial discrepancy between H&E and positron imaging was not investigated. (3) Although the animals were treated with anti-inflammation after the surgery, the unspecific inflammatory [^{18}F]FDG uptake cannot be excluded [38, 39]. (4) Here we made quantitative assessment about the co-registration accuracy to compare imaging modalities. However, there are other factors that might cause not such a good correlation such as e.g., field inhomogeneities in MRI, and this was not evaluated in the study.

(5) Although the MIMI system has the potential of longitudinal imaging, we did not verify this potential yet.

Conclusions

A MIMI system was developed for tumour transpathology. The system provides an imaging tool combining three imaging modalities (positron imaging, MRI, fluorescence imaging). The accurate co-registration of the images obtained from the multi-scale imaging modalities ensures a comprehensive view of the tumour microenvironment. This system can bridge the discrepancies between macroscopic and microscopic images and between in vivo and in vitro images and provides a tool for the regional investigation and longitudinal observation of the underlying physiology within intact tumour tissues.

Declarations

Abbreviations

[¹⁸F]FDG: 2-deoxy-2-(¹⁸F)fluoro-D-glucose

AFN: Atipamezole/flumazenil/naloxone

BLI: Bioluminescence imaging

CCD: Charge-coupled device

DCE-MRI: Dynamic contrast-enhanced magnetic resonance imaging

FITC-dextran: Fluorescein isothiocyanate-dextran

Gd-DTPA: Gadolinium-diethylenetriamine penta-acetic acid

GFP: Green fluorescent protein

H&E: Haematoxylin-eosin

MIMI: Multimodal intravital molecular imaging

MMF: Midazolam/medetomidine/fentanyl

MR: Magnetic resonance

MRI: Magnetic resonance imaging

NEX: Number of excitation

NIR: Near-infrared

PD: Pharmacodynamics

PEEK: Polyetheretherketone

PET: Positron emission tomography

p.i.: Post injection

PK: Pharmacokinetics

RF: Radio frequency

s.c.: Subcutaneously

TRICKS: Time-resolved imaging of contrast kinetics

Acknowledgements

The authors thank Dr. Florian Gärtner, Dr. Anne-Kathrin v. Thaden, Dr. Sabine Schwamberger, Susanne Swirczek and Miriam Mohring for taking care of the animals and helping animal experiments. The authors thank Dr. Christine Bayer, Birgit Blechert, Dr. Daniela Schilling for providing cell lines, Prof. Markus Essler for helpful discussions, Dr. Jan Tous (CRYTUR, spol. s r.o.) for help related to the positron camera.

Funding

The research leading to these results is based on the funding from German Research Foundation (DFG) Collaborative Research Centre 824 (SFB824) and supported by China Scholarship Council. The scientific collaboration between UCLA and TUM was supported by BaCaTec (Project 17, 2012-1).

Availability of data and materials

The datasets used and/or analysed during the current study are available from the corresponding author on reasonable request.

Ethics approval and consent to participate

All the animal studies were approved by the local governmental committee for animal protection and welfare (Tierschutzbehörde, Regierung von Oberbayern, with license protocol number 18-13).

References

1. Tian M, He X, Jin C, He X, Wu S, Zhou R, et al. Transpathology: molecular imaging-based pathology. *European journal of nuclear medicine and molecular imaging*. 2021. doi:10.1007/s00259-021-05234-1.
2. Phelps M, Schwaiger M, Chiti A. Multi-scale imaging as an essential tool for precision medicine. *European Journal of Nuclear Medicine and Molecular Imaging*. 2021. doi:10.1007/s00259-021-05367-3.
3. Cho H, Ackerstaff E, Carlin S, Lupu ME, Wang Y, Rizwan A, et al. Noninvasive multimodality imaging of the tumor microenvironment: registered dynamic magnetic resonance imaging and positron emission tomography studies of a preclinical tumor model of tumor hypoxia. *Neoplasia*. 2009;11:247-59.
4. Bali MA, Metens T, Denolin V, Delhaye M, Demetter P, Closset J, et al. Tumoral and nontumoral pancreas: correlation between quantitative dynamic contrast-enhanced MR imaging and histopathologic parameters. *Radiology*. 2011;261:456-66. doi:10.1148/radiol.11103515.
5. Hu S, Balakrishnan A, Bok RA, Anderton B, Larson PE, Nelson SJ, et al. ¹³C-pyruvate imaging reveals alterations in glycolysis that precede c-Myc-induced tumor formation and regression. *Cell metabolism*. 2011;14:131-42. doi:10.1016/j.cmet.2011.04.012.
6. Viel T, Talasila KM, Monfared P, Wang J, Jikeli JF, Waerzeggers Y, et al. Analysis of the growth dynamics of angiogenesis-dependent and -independent experimental glioblastomas by multimodal small-animal PET and MRI. *Journal of nuclear medicine : official publication, Society of Nuclear Medicine*. 2012;53:1135-45. doi:10.2967/jnumed.111.101659.
7. Jain RK. The next frontier of molecular medicine: delivery of therapeutics. *Nature medicine*. 1998;4:655-7.
8. Puri T, Chalkidou A, Henley-Smith R, Roy A, Barber PR, Guerrero-Urbano T, et al. A method for accurate spatial registration of PET images and histopathology slices. *EJNMMI research*. 2015;5:64. doi:10.1186/s13550-015-0138-7.
9. Jain RK, Munn LL, Fukumura D. Transparent Window Models and Intravital Microscopy: Imaging Gene Expression, Physiological Function and Therapeutic Effects in Tumors. In: Teicher BA, editor. *Tumor Models in Cancer Research*: Springer; 2011.
10. Pittet MJ, Weissleder R. Intravital Imaging. *Cell*. 2011;147:983-91. doi:10.1016/j.cell.2011.11.004.
11. Oishi H, Sunamura M, Egawa S, Motoi F, Unno M, Furukawa T, et al. Blockade of delta-like ligand 4 signaling inhibits both growth and angiogenesis of pancreatic cancer. *Pancreas*. 2010;39:897-903. doi:10.1097/MPA.0b013e3181ce7185.
12. Chen X, Leischner U, Rochefort NL, Nelken I, Konnerth A. Functional mapping of single spines in cortical neurons in vivo. *Nature*. 2011;475:501-5. doi:10.1038/nature10193.
13. Jain RK, Munn LL, Fukumura D. Dissecting tumour pathophysiology using intravital microscopy. *Nature reviews Cancer*. 2002;2:266-76. doi:10.1038/nrc778.

14. Vajkoczy P, Ullrich A, Menger MD. Intravital fluorescence videomicroscopy to study tumor angiogenesis and microcirculation. *Neoplasia*. 2000;2:53-61. doi:DOI 10.1038/sj.neo.7900062.
15. Guba M, von Breitenbuch P, Steinbauer M, Koehl G, Flegel S, Hornung M, et al. Rapamycin inhibits primary and metastatic tumor growth by antiangiogenesis: involvement of vascular endothelial growth factor. *Nature medicine*. 2002;8:128-35. doi:10.1038/nm0202-128.
16. Dewhirst MW, Ong ET, Braun RD, Smith B, Klitzman B, Evans SM, et al. Quantification of longitudinal tissue pO₂ gradients in window chamber tumours: impact on tumour hypoxia. *Brit J Cancer*. 1999;79:1717-22.
17. Cardenas-Navia LI, Mace D, Richardson RA, Wilson DF, Shan S, Dewhirst MW. The pervasive presence of fluctuating oxygenation in tumors. *Cancer research*. 2008;68:5812-9. doi:10.1158/0008-5472.CAN-07-6387.
18. Gaustad JV, Brurberg KG, Simonsen TG, Mollatt CS, Rofstad EK. Tumor vascularity assessed by magnetic resonance imaging and intravital microscopy imaging. *Neoplasia*. 2008;10:354-62. doi:10.1593/neo.08162.
19. Schafer R, Leung HM, Gmitro AF. Multi-modality imaging of a murine mammary window chamber for breast cancer research. *BioTechniques*. 2014;57:45-50. doi:10.2144/000114191.
20. Laschke MW, Vollmar B, Menger MD. The dorsal skinfold chamber: window into the dynamic interaction of biomaterials with their surrounding host tissue. *Eur Cell Mater*. 2011;22:147-64.
21. Gregory MP, Andrew NF, Siqing S, Gabi H, Guoqing Z, Cassandra LF, et al. In vivo optical molecular imaging and analysis in mice using dorsal window chamber models applied to hypoxia, vasculature and fluorescent reporters. *Nat Protoc*. 2011;6:1355-66. doi:10.1038/nprot.2011.349.
22. Wang Q, Tous J, Liu Z, Ziegler S, Shi K. Evaluation of Timepix silicon detector for the detection of 18F positrons. *J Instrument*. 2014;9:C05067.
23. Wang Q, Liu Z, Ziegler SI, Shi K. Enhancing spatial resolution of (18)F positron imaging with the Timepix detector by classification of primary fired pixels using support vector machine. *Physics in medicine and biology*. 2015;60:5261-78. doi:10.1088/0031-9155/60/13/5261.
24. Romano A, Tavanti F, Rossi Espagnet MC, Terenzi V, Cassoni A, Suma G, et al. The role of time-resolved imaging of contrast kinetics (TRICKS) magnetic resonance angiography (MRA) in the evaluation of head-neck vascular anomalies: a preliminary experience. *Dento maxillo facial radiology*. 2015;44:20140302. doi:10.1259/dmfr.20140302.
25. Damon J. Properties of Ridges and Cores for Two-Dimensional Images. *J Math Imaging Vis*. 1999;10:163-74. doi:10.1023/A:1008379107611.
26. Wehrl HF, Sauter AW, Divine MR, Pichler BJ. Combined PET/MR: a technology becomes mature. *J Nucl Med*. 2015;56:165-8. doi:10.2967/jnumed.114.150318.
27. Hundshammer C, Braeuer M, Muller CA, Hansen AE, Schillmaier M, Duwel S, et al. Simultaneous characterization of tumor cellularity and the Warburg effect with PET, MRI and hyperpolarized (13)C-MRSI. *Theranostics*. 2018;8:4765-80. doi:10.7150/thno.25162.
28. Fanti S, Minozzi S, Antoch G, Banks I, Briganti A, Carrio I, et al. Consensus on molecular imaging and theranostics in prostate cancer. *The lancet oncology*. 2018;19:e696-e708. doi:10.1016/S1470-2045(18)30604-1.
29. Gennaro N, Marrari A, Renne SL, Cananzi FCM, Quagliuolo VL, Di Brina L, et al. Multimodality imaging of adult rhabdomyosarcoma: the added value of hybrid imaging. *The British journal of radiology*. 2020;93:20200250. doi:10.1259/bjr.20200250.

30. Catalano OA, Horn GL, Signore A, Iannace C, Lepore M, Vangel M, et al. PET/MR in invasive ductal breast cancer: correlation between imaging markers and histological phenotype. *British journal of cancer*. 2017;116:893-902. doi:10.1038/bjc.2017.26.
31. Preibisch C, Shi K, Kluge A, Lukas M, Wiestler B, Gottler J, et al. Characterizing hypoxia in human glioma: A simultaneous multimodal MRI and PET study. *NMR in biomedicine*. 2017;30. doi:10.1002/nbm.3775.
32. Gaustad JV, Brurberg KG, Simonsen TG, Mollatt CS, Rofstad EK. Tumor vascularity assessed by magnetic resonance imaging and intravital microscopy imaging. *Neoplasia*. 2008;10:354-62.
33. Berker Y, Li Y. Attenuation correction in emission tomography using the emission data-- A review. *Med Phys*. 2016;43:807-32. doi:10.1118/1.4938264.
34. Vaquero JJ, Kinahan P. Positron Emission Tomography: Current Challenges and Opportunities for Technological Advances in Clinical and Preclinical Imaging Systems. *Annual review of biomedical engineering*. 2015;17:385-414. doi:10.1146/annurev-bioeng-071114-040723.
35. Liu Z, Jian Z, Wang Q, Cheng T, Feurecker B, Schwaiger M, et al. A continuously infused microfluidic radioassay system for the characterization of cellular pharmacokinetics. *J Nucl Med*. 2016;57:1548-55. doi:10.2967/jnumed.115.169151.
36. Hofheinz F, Langner J, Petr J, Beuthien-Baumann B, Oehme L, Steinbach J, et al. A method for model-free partial volume correction in oncological PET. *EJNMMI Research*. 2012;2:16. doi:10.1186/2191-219X-2-16.
37. Cysouw MCF, Golla SVS, Frings V, Smit EF, Hoekstra OS, Kramer GM, et al. Partial-volume correction in dynamic PET-CT: effect on tumor kinetic parameter estimation and validation of simplified metrics. *EJNMMI Research*. 2019;9:12. doi:10.1186/s13550-019-0483-z.
38. Sadeghi MM. (18)F-FDG PET and vascular inflammation: time to refine the paradigm? *J Nucl Cardiol*. 2015;22:319-24. doi:10.1007/s12350-014-9917-1.
39. Kim M, Achmad A, Higuchi T, Arisaka Y, Yokoo H, Yokoo S, et al. Effects of intratumoral inflammatory process on 18F-FDG uptake: pathologic and comparative study with 18F-fluoro- α -methyltyrosine PET/CT in oral squamous cell carcinoma. *J Nucl Med*. 2015;56:16-21. doi:10.2967/jnumed.114.144014.

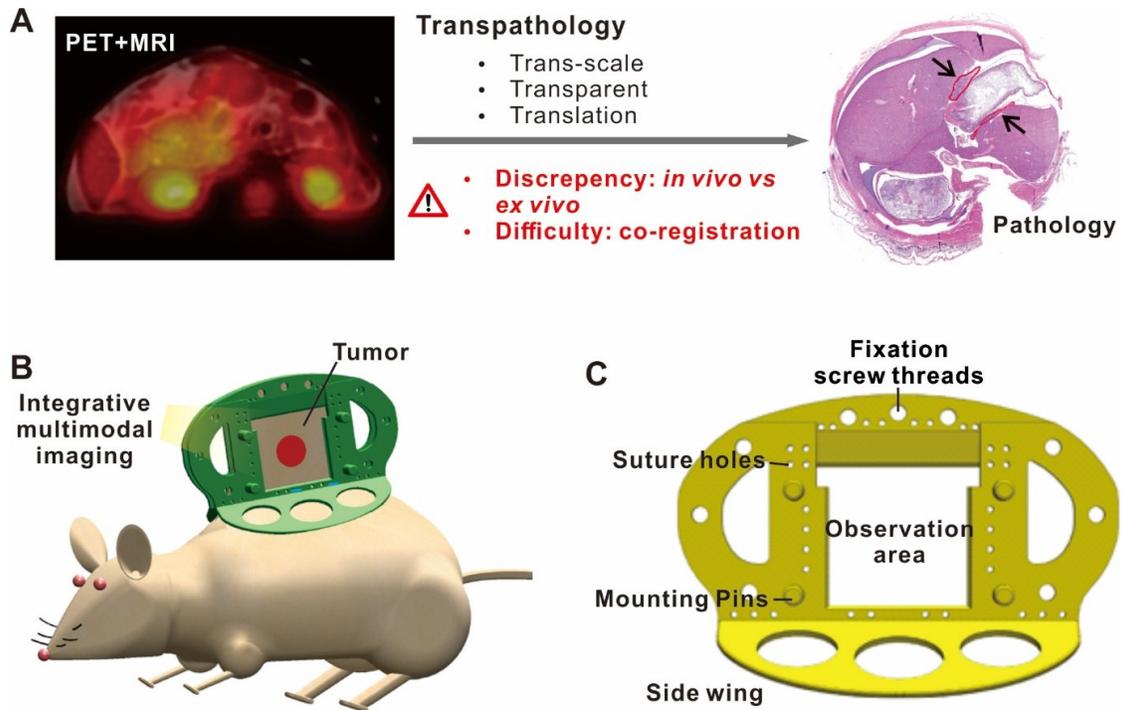


Fig. 1 (A) The concept of transpathology research and its challenges; (B) A concept of integrative MIMI system based on animal model with dorsal skin window chamber for transpathology investigation, which enables positron imaging, MRI and optical imaging within the same intact framework; (C) A detailed sketch of the designed dorsal skin window chamber with mounting pins to fix a positron camera and optical coordinate system, fixation screw threads, and suture holes as further fiducial markers for localization with imaging such as MRI.

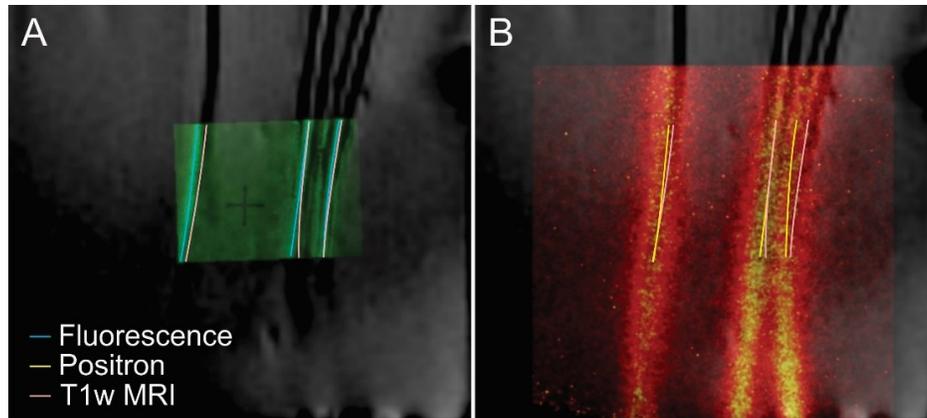


Fig. 2 An exemplary fused image of MRI, positron, and fluorescence imaging of a phantom with three catheters. The catheters were first filled with [^{18}F]FDG for positron imaging, then filled with FITC-dextran for fluorescence imaging and finally filled with water for MRI imaging. (A) fusion of fluorescence imaging with T1w MRI; (B) fusion of positron imaging with T1w MRI. The lines of different colors denote the skeletons of signals of the catheters in the corresponding imaging modalities.

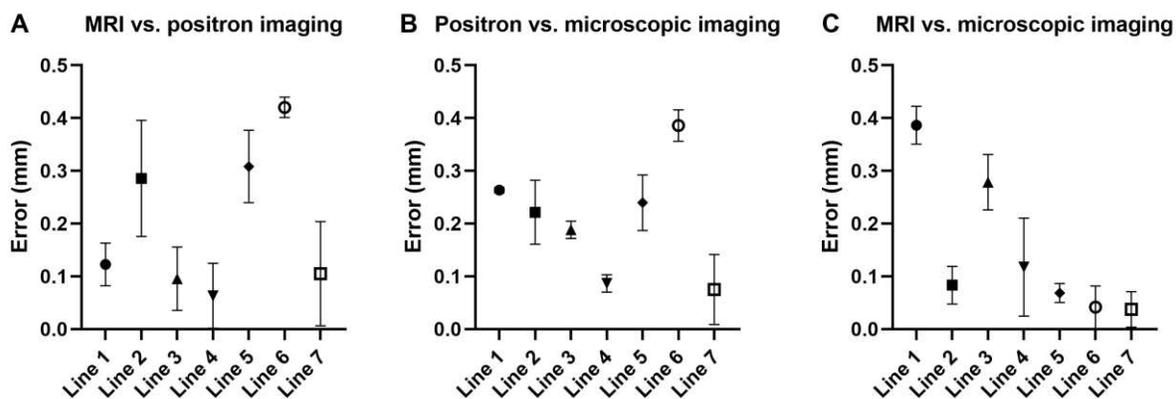


Fig. 3 The co-registration position error between the three imaging modalities of all imaged catheters (skeleton lines 1-7). The absolute distance between pairs of points along the skeleton lines are plotted for each line, and the mean and SD are plotted. (A) MRI and positron images; (B) Positron and microscopy images; (C) MRI and microscopy images.

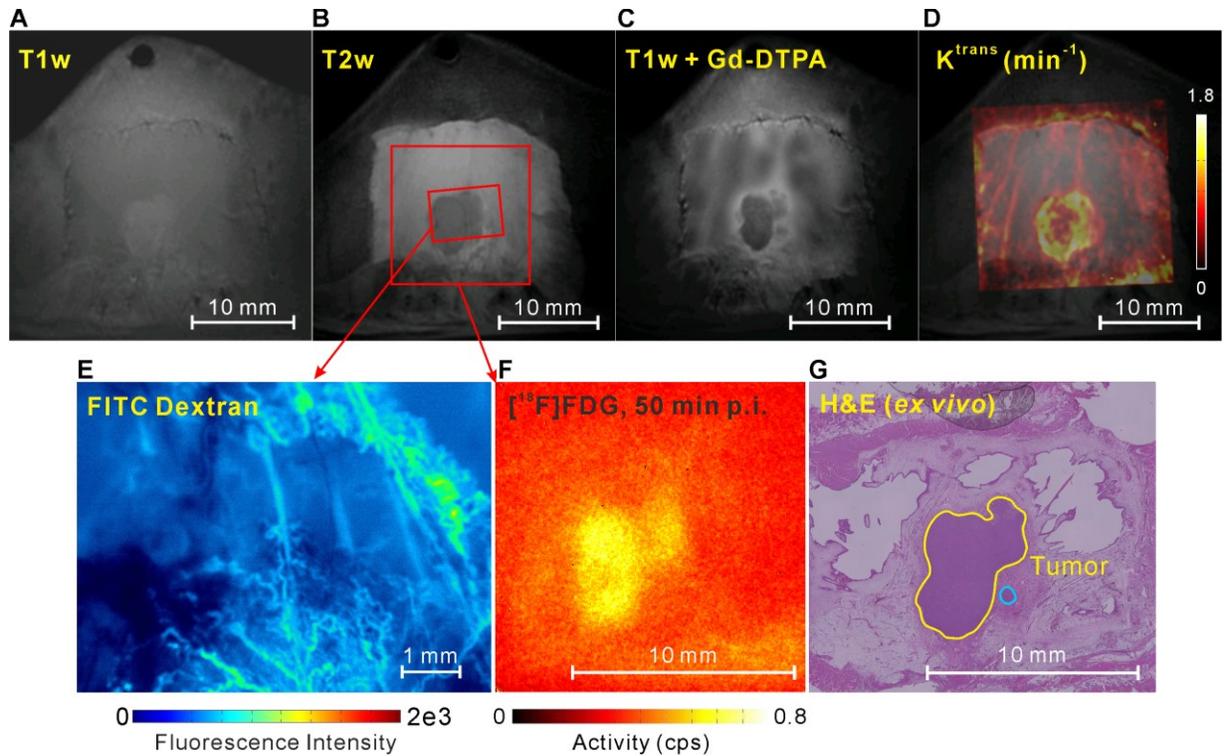


Fig. 4 Example imaging results of the multimodal intravital molecular imaging system: (A) a T1 weighted MR image, (B) a T2 weighted MR image, (C) a T1 weighted MR image after Gd-DTPA injection, (D) the K^{trans} map of the MR image; (E) a FITC-Dextran fluorescence image, (F) an $[^{18}\text{F}]\text{FDG}$ positron image; and (G) an H&E staining slice of the tumour and periphery tissue. For E and F, the locations of the images were delineated with the red boxes in (B) and linked with red arrows. In G, yellow and blue outlines depict the tumour locations in the tissue. Note the H&E image was manually co-registered to the in vivo images without the support fiducial markers.

Figures

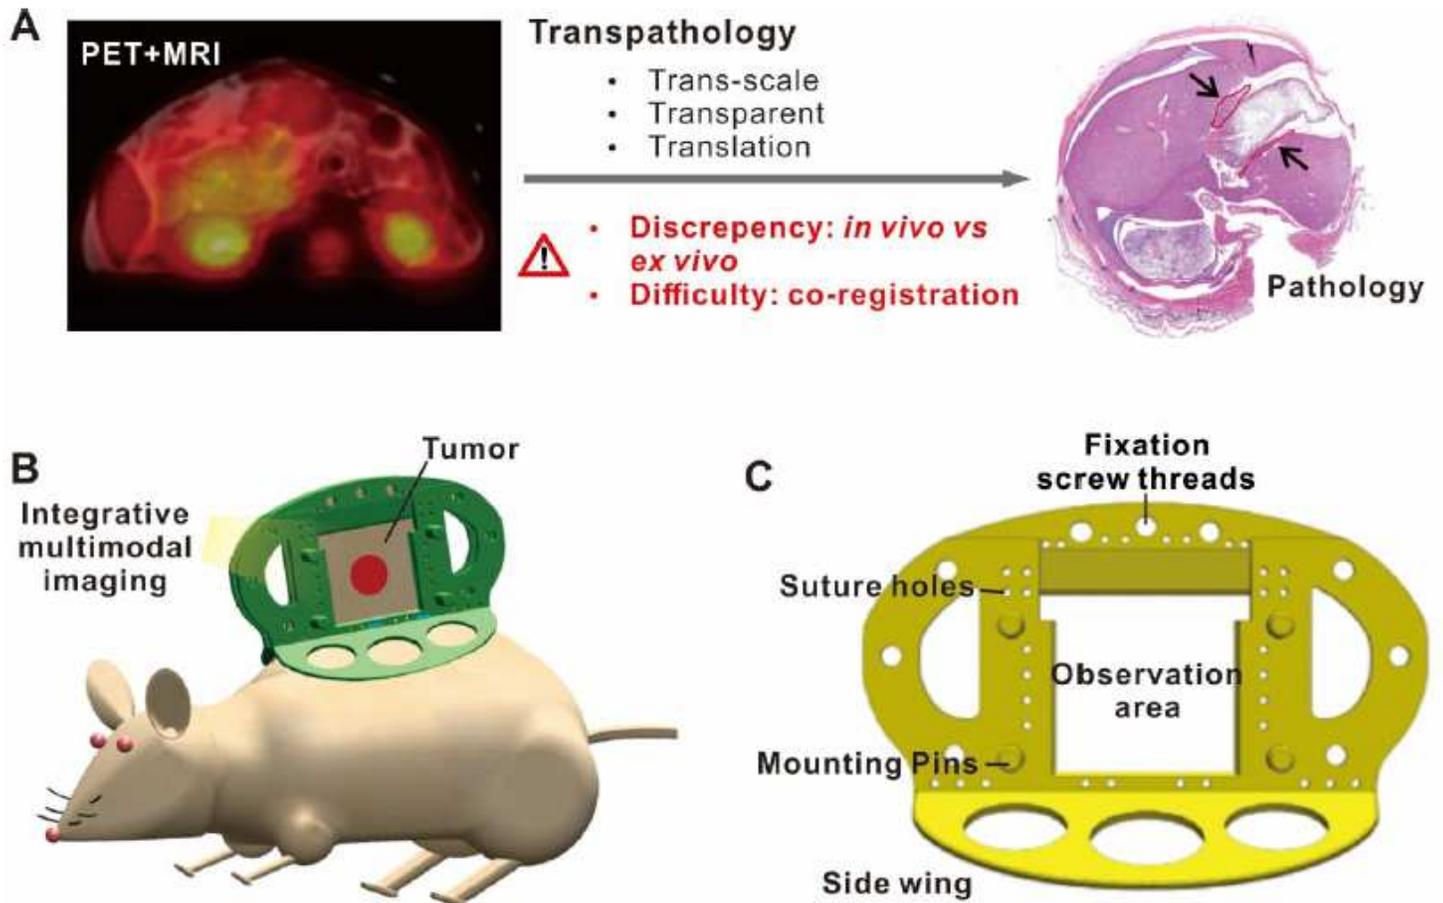


Figure 1

(A) The concept of transpathology research and its challenges; (B) A concept of integrative MIMI system based on animal model with dorsal skin window chamber for transpathology investigation, which enables positron imaging, MRI and optical imaging within the same intact framework; (C) A detailed sketch of the designed dorsal skin window chamber with mounting pins to fix a positron camera and optical coordinate system, fixation screw threads, and suture holes as further fiducial markers for localization with imaging such as MRI.

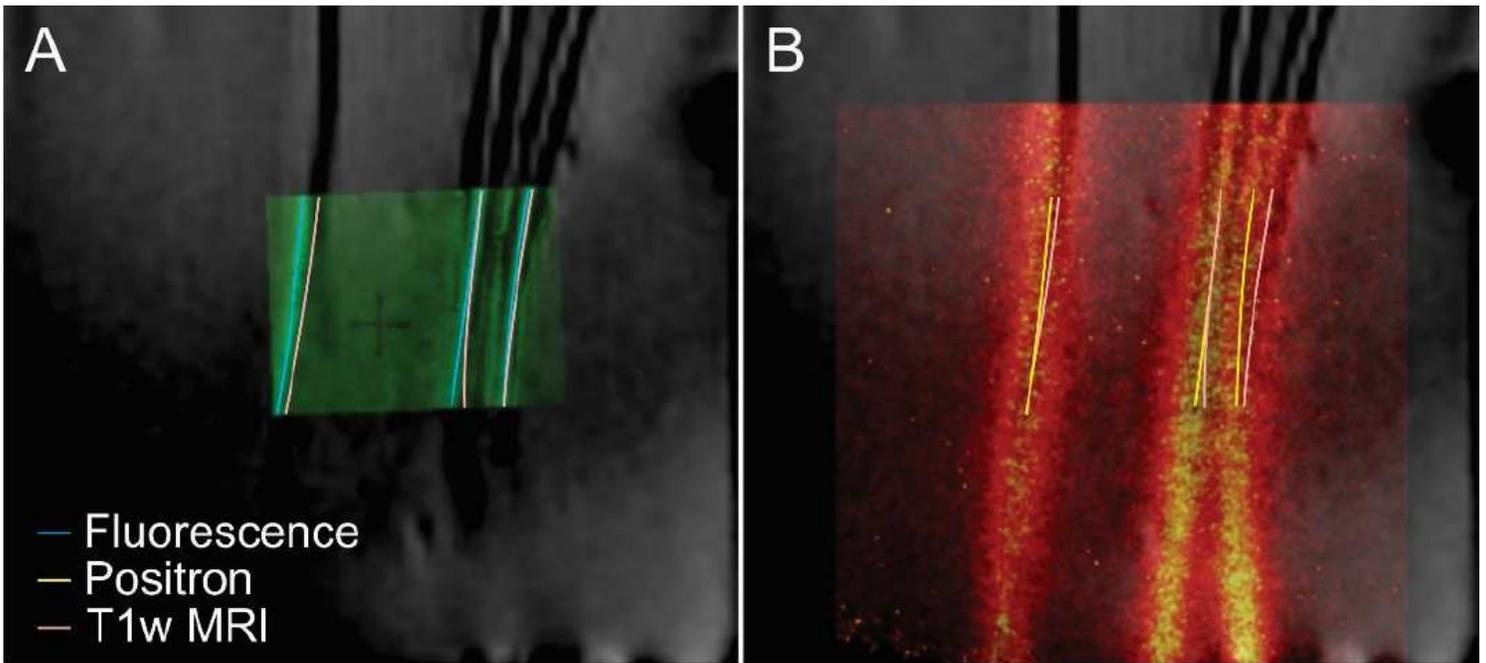


Figure 2

An exemplary fused image of MRI, positron, and fluorescence imaging of a phantom with three catheters. The catheters were first filled with $[^{18}\text{F}]\text{FDG}$ for positron imaging, then filled with FITC-dextran for fluorescence imaging and finally filled with water for MRI imaging. (A) fusion of fluorescence imaging with T1w MRI; (B) fusion of positron imaging with T1w MRI. The lines of different colors denote the skeletons of signals of the catheters in the corresponding imaging modalities.

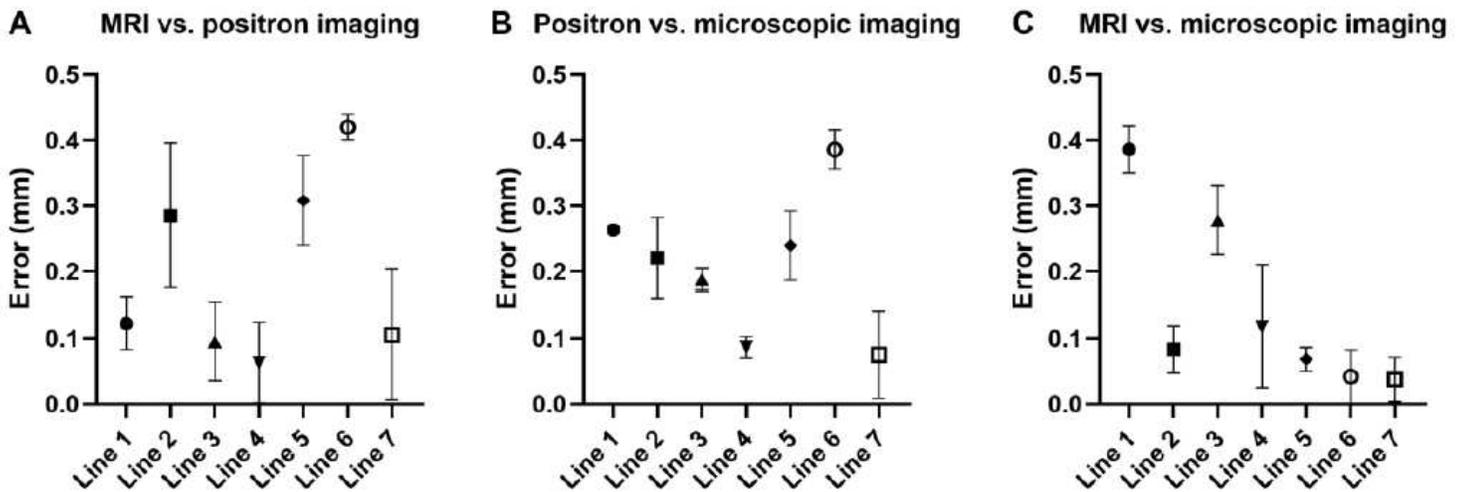


Figure 3

The co-registration position error between the three imaging modalities of all imaged catheters (skeleton lines 1-7). The absolute distance between pairs of points along the skeleton lines are plotted for each line, and the mean and SD are plotted. (A) MRI and positron images; (B) Positron and microscopy images; (C) MRI and microscopy images.

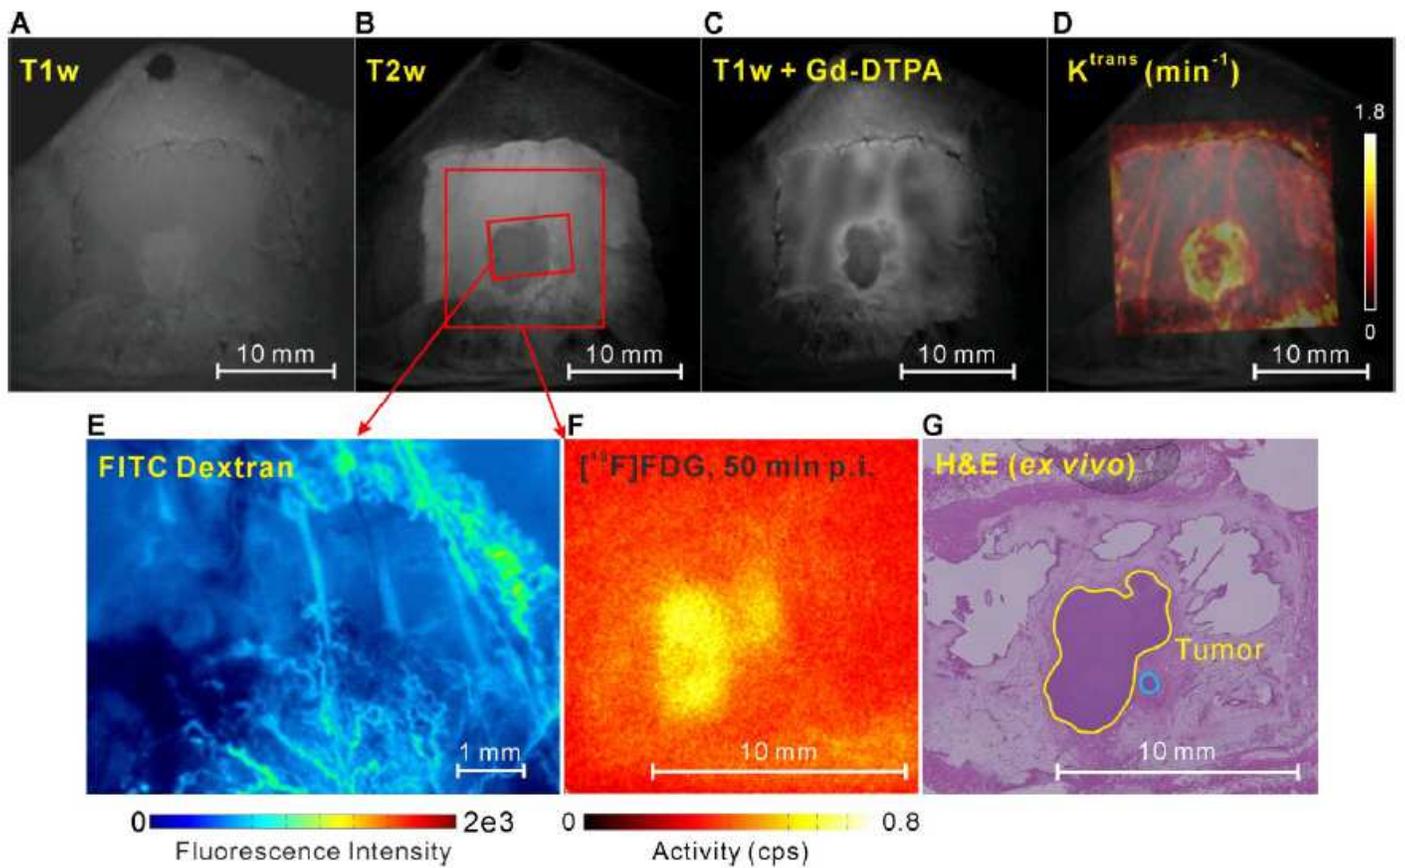


Figure 4

Example imaging results of the multimodal intravital molecular imaging system: (A) a T1 weighted MR image, (B) a T2 weighted MR image, (C) a T1 weighted MR image after Gd-DTPA injection, (D) the K^{trans} map of the MR image; (E) a FITC-Dextran fluorescence image, (F) an $[^{18}F]FDG$ positron image; and (G) an H&E staining slice of the tumour and periphery tissue. For E and F, the locations of the images were delineated with the red boxes in (B) and linked with red arrows. In G, yellow and blue outlines depict the tumour locations in the tissue. Note the H&E image was manually co-registered to the in vivo images without the support fiducial markers.

Supplementary Files

This is a list of supplementary files associated with this preprint. Click to download.

- [LiuMultimodalIntravitalImagingSupplementalMaterials.pdf](#)