

An open source extrusion bioprinter based on the E3D motion system and tool changer to enable FRESH and multi-material bioprinting

Adam Engberg

Uppsala University

Christina Stelzl

Uppsala University

Olle Eriksson

Uppsala University

Paul O'Callaghan

Uppsala University

Johan Kreuger (✉ johan.kreuger@mcb.uu.se)

Uppsala University

Research Article

Keywords: Bioprinting, open source bioprinter, FRESH, cancer cells, collagen, E3D motion system and tool changer

Posted Date: June 23rd, 2021

DOI: <https://doi.org/10.21203/rs.3.rs-653725/v1>

License:  This work is licensed under a Creative Commons Attribution 4.0 International License.

[Read Full License](#)

An open source extrusion bioprinter based on the E3D motion system and tool changer to enable FRESH and multi-material bioprinting

Adam Engberg¹, Christina Stelzl¹, Olle Eriksson¹, Paul O'Callaghan¹, and Johan Kreuger^{1*}

¹Department of Medical Cell Biology, Uppsala University, Uppsala, Sweden

*Corresponding author
E-mail: johan.kreuger@mcb.uu.se

Abstract

Bioprinting is increasingly used to create complex tissue constructs for an array of research applications, and there are also increasing efforts to print tissues for transplantation. Bioprinting may also prove valuable in the context of drug screening for personalized medicine for treatment of diseases such as cancer. However, the rapidly expanding bioprinting research field is currently limited by access to bioprinters. To increase the availability of bioprinting technologies we present here an open source extrusion bioprinter based on the E3D motion system and tool changer to enable high-resolution multi-material bioprinting. As proof of concept, the bioprinter is used to create collagen constructs using freeform reversible embedding of suspended hydrogels (FRESH) methodology, as well as multi-material constructs composed of distinct sections of laminin and collagen. Data is presented demonstrating that the bioprinted constructs support growth of cells either seeded onto printed constructs or included in the bioink prior to bioprinting. This open source bioprinter is easily adapted for different bioprinting applications, and additional tools can be incorporated to increase the capabilities of the system.

Keywords: Bioprinting, open source bioprinter, FRESH, cancer cells, collagen, E3D motion system and tool changer

Introduction

Additive manufacturing is an umbrella term for a variety of manufacturing techniques usually based on building three-dimensional (3D) objects in a layer-by-layer fashion. Additive technologies are gaining widespread popularity in a variety of research fields, as well as in industry, as 3D printing enables rapid prototyping and generation of objects with complex geometries from a very wide range and combination of materials. Bioprinting describes the application of additive manufacturing to reproducibly create tissue-like 3D constructs composed of biomolecules and/or biomaterials and cells. As a tissue engineering technology, bioprinting permits cells to be incorporated into printed constructs post-production or during the printing process, and the ultimate goal is often to recapitulate the architecture and function of living tissues and organs^{1,2}. Such constructs present opportunities to study cell biology and pathogenic processes in complex, well-defined environments. Bioprinted constructs also hold potential to become widely used model systems and assays for drug screening³⁻⁵, and their viability as transplantable materials for patient care is an area of intense research interest⁶⁻⁹.

Developments in the field of bioprinting encompasses many established fields of research such as material science, cell and tissue engineering, regenerative medicine, as well as

robotics, automation and biotechnology. This requirement for interdisciplinary collaborations presents a number of challenges to progress in the bioprinting field; however, by increasing the availability of open source and user-friendly bioprinter solutions, more researchers are likely to adopt the technology and in doing so advance the field as a whole. As with standard additive manufacturing, many different technologies are capable of constructing bioprinted 3D-objects in a layer-by-layer fashion. The most commonly used techniques for the printing of cell-laden bioinks are extrusion-based bioprinting¹⁰, laser-assisted bioprinting, stereolithography, and inkjet-based bioprinting¹¹. To date extrusion based bioprinting is one of the most widespread techniques, which has borrowed innovations from the analogous fused filament fabrication (FFF) technology that is extensively used in plastic additive manufacturing. Compared to other bioprinting technologies, extrusion based bioprinting has several advantages such as low cost, a relatively high printing speed, and compatibility with bioinks in a wide range of viscosities. However, extrusion-based bioprinting does suffer from a relatively low spatial resolution, and cell viability can be compromised due to the mechanical stress generated during extrusion of cells through the deposition needle or nozzle¹².

A challenge that confronts many additive manufacturing techniques, especially those using soft materials such as hydrogels, is the low structural stability of the construct during the printing process, which can negatively impact the geometry and architecture of the intended construct design. Strategies that have been employed to circumvent this limitation include the use of sacrificial support materials. This allows for a construct to be printed in one or more bioinks of choice, while it is simultaneously embedded in a structurally supportive scaffold material printed in parallel. Once the construct is complete and stabilized through post-printing reactions or treatments, the sacrificial material can be removed to release the construct. This technique can also be used to introduce design features such as channels that facilitate the perfusion of printed constructs^{13,14}. However, this strategy employing sacrificial materials typically demands a bioprinting platform with the capacity to perform multi-material printing. However, freeform reversible embedding of suspended hydrogels (FRESH) is an innovative solution that provides a 3D structurally supportive print environment, without the need for multi-material printer functionality^{15,16}. During FRESH bioprinting, collagen-based bioinks (or other bioinks of interest) are extruded directly into a support bath consisting of gelatin microparticles, and this permits complex 3D constructs to be printed in an essentially suspended state, without the need for printed support structures. The gelatin bath can subsequently be melted away by increasing the temperature, allowing the construct to be retrieved. The FRESH bioprinting strategy has been widely adopted throughout the bioprinting research community¹⁷; therefore, designing bioprinting platforms that are compatible with FRESH bioprinting will likely be of great general interest.

Efforts to bring bioprinters to a wider audience have included the repurposing of affordable FFF-printers for bioprinting applications^{18,19}, and while they may be limited to the extrusion of a single type of bioink at a time, previous studies demonstrate the benefits of leveraging existing additive manufacturing technologies for bioprinting. In the present study we present an open source extrusion-based bioprinter built around the E3D motion system and tool changer, with the potential to produce constructs using up to four syringe pump tools and bioinks. The bioprinter features a transparent polycarbonate cabinet with an integrated HEPA filter and air intake fan to enable contamination-free bioprinting, and automatic tool offset calibration and bed leveling, making it easy to use multiple syringe pump tools to combine different bioinks in order to create complex bioprinted 3D constructs. Due to the open source nature of the components used, the system is highly adaptable to allow for incorporation of

new tools and functionalities. FRESH bioprinting as well as multi-material printing with collagen and laminin was performed to demonstrate the capacity of the system.

Results and discussion

Bioprinter assembly

The open source extrusion bioprinter was built around the E3D motion system and tool changer, and fitted with custom-built syringe pump tools (Fig. 1a). The E3D motion system is easily configurable and delivers robust and precise motion control²⁰. E3D provides free access to the systems build files²¹, which facilitated the design process when adapting the existing system for the bioprinting purpose described here. A polycarbonate box fitted with an integrated HEPA filter and air intake fan was constructed to enclose the E3D system to reduce the risk of contamination of bioprinted constructs. The polycarbonate enclosure could easily be adapted to allow for temperature and humidity control should this be required for future bioprinting applications (Fig. 1b). The tool changer retrieves tools (in this case syringe pumps) from four positions at the back of the motion system frame, and these tools together enable multi-material printing. The motion system controls the tools x and y positions²⁰, and the print platform is operated separately and translated along the z-axis. A web camera for x- and y-axis calibration and microswitch for z-axis calibration was mounted on the print platform to enable accurate spatial alignment of tools after tool exchange (Fig. 1a, b), and a calibration protocol was operated via a side-mounted touchscreen display.

Syringe pump extrusion tool design and assembly

The custom-built syringe pump extrusion tools was built around a stepper motor that linearly translates an integrated lead screw (Fig. 2a). The stepper motor was mounted on top of a 3D-printed plunger housing with an attached E3D tool mount at the back of the housing (Fig. 2a and b). The end of the lead screw was fitted with a plunger press (most clearly seen in Fig. 2b, exploded view), which applies force to the syringe plunger to extrude bioinks (hydrogels) from the syringe. The plunger housing was in turn attached to the top of a 3D-printed syringe mount (Fig. 2b). The syringe mounts can easily be designed to hold either 0.25, 1, or 5 ml Hamilton gastight syringes, or 5 ml BD syringes, and are compatible with the extrusion of bioinks through different needles or nozzle attachments. Notably, the minimum volume of dispensed bioink is dependent on both the inner diameter of the selected syringe and the micro-stepping setting of the stepper motor. The syringe mounts were equipped with three adjustable thumbscrews, which allowed the syringe to be centrally positioned in the mount to ensure perpendicular alignment to the build platform. Importantly, the custom built syringe pump presented here shares similarities with and is in part adapted from previously proposed solutions²², where the versatility afforded by accommodating different syringe types has also been demonstrated²³.

FRESH bioprinting of collagen constructs

As the FRESH bioprinting method has been widely adopted by the bioprinting research community, we assessed its implementation on the present open source bioprinter platform. A cuboid construct was designed using Autodesk Fusion 360. It consisted of five square layers with a tool path that printed the infill as a continuous line, which for each layer followed a series of diagonal, parallel paths (Fig. 3a). The direction of the diagonal print path rotated by 90° between layers, which produced the crisscrossed lattice appearance seen in the final FRESH printed part, which had similar dimensions to those of the intended design (Fig. 3b). The construct was printed using a collagen-based bioink (Collagen Ink 240) in a FRESH

LifeSupport gelatin support bath. To facilitate ease of handling, the construct was printed within a custom-made 3D printed polyetherketoneketone (PEKK) basket, which was manually removed from the support bath to permit transfer of the construct for melting of the gelatin microparticles, and subsequent washing of the released construct (Fig. 3b). It has previously been demonstrated that the gelatin microparticles in the FRESH support bath imprint topological indentations in the collagen surfaces of the printed constructs¹⁶. Here, confocal microscopy z-stack imaging of Col-F stained FRESH bioprinted constructs confirmed the presence of similar microparticle dimples on the surface of the collagen constructs produced using the open source bioprinter (Fig. 3c). These depressions are likely advantageous for cell seeding as they present craters on the surface of the constructs, which trap cells seeded in suspensions and promote cell attachment followed by infiltration of the constructs.

Viability of cells grown on bioprinted collagen constructs

Individual FRESH bioprinted collagen constructs were moved into wells of a chambered coverslip with a glass bottom compatible with high resolution microscopy. MDA-MB-231 breast cancer cells were seeded onto the collagen constructs, or for comparison were seeded into wells without constructs, where after the cells were cultured for 20 h. Staining of cells to visualize the cytoskeleton as well as cell nuclei identified cells that had attached to the collagen construct and adopted normal cell morphology (Fig. 3d). To assess the viability of cells seeded in the bioprinted collagen constructs, as compared to cells grown in conventional glass bottom culture chambers, cells were incubated with the Cellevant caspase 3/7 detection reagent that reports on apoptosis, and propidium iodide, which detects the presence of dead cells. Individual cells were identified by the nuclear stain NucBlue, and the potent apoptosis-inducer staurosporine was used as a positive control to confirm that this strategy for assessing viability was reliable. Importantly, there was no difference between the degree of apoptosis (Fig. 3e) or presence of dead cells (Fig. 3f) in cells grown in the glass-bottomed wells compared to those seeded into the bioprinted collagen constructs. However, cells seeded on the collagen constructs were more sensitive to staurosporine-induced apoptosis and death than those seeded in the glass-bottomed wells (Fig. 3e and f), and while these differences were small it highlights the impact that a 3D environment can have on cell survival in the presence of specific drugs.

Viability of cells extruded in laminin bioink

Extrusion of cell-laden bioinks circumvents certain problems associated with the seeding of constructs with cells post bioprinting. Firstly, the distribution of cells in the construct is typically more homogenous, and at least for thicker constructs, the ability of cells to migrate within and penetrate into the depths of such constructs will not be a limiting factor. In addition, it is difficult to precisely control the spatial distribution of different specific cell types in a complex construct by cell seeding after bioprinting. Instead, constructs can be composed of independently extruded hydrogels each containing specific cell types of interest. However, extrusion of cell-containing hydrogels exerts shear stress on the cells to reduce cell viability¹². Here, we determined to assess the viability of MDA-MB-231 cells after they had been extruded in laminin bioink either through an 18 G nozzle or an 18 G needle as compared to the viability of cells that had simply been dispersed in the bioink. Cell viability was assessed by a live/dead staining protocol employing propidium iodide and fluorescein diacetate (Fig. 4a), and it could be seen that extrusion during bioprinting did not reduce cell viability (Fig. 4b).

Multi-material bioprinting

The capacity of a bioprinter to produce constructs composed of two or more materials presents important advantages for construct design. For example, combining a network of sacrificial materials (e.g. Pluronic F127) into a hydrogel construct, which is removed after printing, can provide perfusion channels, which can increase cell viability and survival in larger constructs²⁴. Furthermore, combining bioinks in controlled ratios to reproducibly create experimental tissue culture environments, enables studies of cell responses in which the role of the surrounding matrix composition or specific treatments can be evaluated²⁵⁻²⁸. To demonstrate the multi-material printing capacity of the open source bioprinter, we designed a square construct intersected by eight spokes originating from the constructs center, to be printed with cell-laden laminin bioink (Fig. 4c, red lines). The spaces between the laminin spokes and the outer boundary of the square were filled with collagen bioink (Fig. 4c green lines). The final print had similar dimensions to the intended design (Fig. 4d). Col-F staining of the collagen ink revealed a defined border between the collagen and laminin regions of the print (Fig. 4e). Unexpectedly, Col-F also stained the MDA-MB-231 cells in the laminin regions of the construct, and like the Celltracker red staining revealed an even distribution of the cells in the laminin bioink (Fig. 4e).

Conclusion and outlook

The open source bioprinter presented here, based on the E3D motion system and tool changer, enables a variety of bioprinting tasks including FRESH bioprinting, multi-material prints, and the extrusion of cell-laden bioinks. In the presented configuration only two of the four tool positions were used. The remaining tool positions present opportunities for further automation of protocols to reduce user intervention, and to increase reproducibility and throughput. For instance, we are currently developing a grip tool and protocol to manipulate the 3D printed basket in which the FRESH collagen constructs are bioprinted, to allow for automated construct transport from the gelatin support bath to a heated washing station, which melts the gelatin support material. The grip tool can subsequently move the construct through additional washing solutions, effectively automating key steps of the post-processing procedure. The benefits of automating biofabrication protocols have been outlined for the formation of tissue spheroids^{29,30}, the analysis of multi-cell type behaviors³¹, and is important for future efforts to facilitate and scale up bioprinting of constructs for use in research and drug screening. The open source bioprinter is easily adapted for different bioprinting applications, and the possibility of incorporating additional tools should accelerate the development of novel bioprinting approaches and applications.

Materials and methods

The open source bioprinter and syringe pump extrusion tool

The bioprinter (Fig. 1) was built around the E3D tool changer and motion system (E3D-online, London, United Kingdom)^{20,21}, and enclosed in a custom-built polycarbonate cabinet with an integrated a HEPA filter with an air intake fan. The syringe pump extrusion tool (Fig. 2) was built using a stepper motor, a lead screw, and 3D-printed plunger housing and syringe holder. All computer-aided design (CAD) was done using Fusion 360 (Autodesk Inc, San Rafael, USA). All 3D-printed parts for the extrusion tools were printed on a Form 3 SLA 3D printer (Formlabs) in standard clear resin or tough 2000 resin (Formlabs) with a Z-resolution of ~100 micrometer. All prints with resin were washed and cured according to the

manufacturer's instructions. The baskets used for handling FRESH-printed constructs were 3D-printed in PEKK-A (Kimya, Nantes, France) on a miniFactory Ultra FFF 3D-printer (miniFactory Oy LTD, Seinäjoki, Finland). Brackets for the enclosure, camera housing, touch screen mount and HEPA-filter holder were printed in PLA (Add North 3D AB, Ölsremma, Sweden) on a Prusa I3 MK3S (Prusa, Prague, Czech Republic). STL-files for all 3D printed components as well as a list of additional bioprinter components required to adapt the E3D toolchanger and motion system and to build the syringe pump extrusion tool are included in the Supplementary Materials section.

Bioprinter operation

Before powering up the printer, the stepper motors driving the syringe pump extrusion tools were connected to the control board and the tools placed in the tool dock. The E3D motion system is controlled by a Duet Wifi controller board together with the expansion board Duex 5. This enables control of up to 10 stepper motors. 4 stepper motors in the E3D motion system are used to control the x-, y- and z-axes as well as the tool changer mechanism. In addition, syringe pump extrusion tools use one stepper motor output each. Configuration of any additional tools are made via modification of the *config.g-file* in the DWC interface. For multi-material prints, requiring the use of two or more tools, calibrations for tool offsets were required as described below.

Tool offset calibration

Tool offset identification was performed using the "Tool Alignment with Machine Vision" (TAMV) program originally developed by Danal Estes (<https://github.com/DanalEstes/TAMV>), using a Logitech web camera mounted on the print platform and a Raspberry Pi 4B running OpenCV. A prerequisite for running the calibration commands is that all axes first are homed. The procedure for x- and y-axis tool offset identification is performed per the instructions on the creator's website. Z-axis offset calibration is facilitated by a microswitch mounted on the build plate, this enables probing of individual tools to identify differences in syringe and needle length. For the calibration to work correctly the leadscrew in the stepper motor must be engaged with the plunger via the plunger press (Fig. 2). This is done by running the "Tool 0 – Select" macro from the "macros" section of DWC, followed by stepwise movement of the leadscrew until it applies pressure to the plunger, which is repeated for each syringe pump tool. The procedure for z-axis offset calibration is performed automatically via a custom-made G-code script, using the spatial positioning of the first tool as the reference for offset calibration for the other tools. The first tool is picked up and positioned with the needle tip above the microswitch, followed by movement of the build plate until the microswitch is engaged. After the reference position of the first tool has been logged, other tools are then picked up and used to trigger the microswitch. At the end of the procedure, a z-offset value is presented in the DWC web interface and can be inserted manually into *config.g* which stores the offset values for each tool. This procedure is repeated between each new print since needle length and position of needle tips in the tool will differ between prints. Once calibration is complete bioprinting can be initiated by using the macro to pick up the loaded tool, manually positioning it at the starting point, zero the z-axis and start the G-code file for the selected construct of interest.

Toolpath generation

The toolpath generation software (Simplify3D, Cincinnati, USA) was used to generate G-code files for bioprinting of the different constructs. Bioprinting was typically performed at a speed of 10 mm/s, and printing parameters are available in a *.fff* file format, which is native to

Simplify3D. Further information about software configuration and slicing settings can be found in the Supplementary Materials section.

Cell culture

The MDA-MB-231 (ATCC) breast cancer cell line was cultured in Dulbecco's Modified Eagle Medium (DMEM) Glutamax (Gibco, Thermo Fisher Scientific, Uppsala, Sweden), supplemented with 10% Fetal Bovine Serum (FBS; Thermo Fisher Scientific), referred to hereafter as culture medium, under standard cell culture conditions in a humidified incubator (5 % CO₂, 37°C).

Bioink loading

The Collagen Ink 240 (Advanced Biomatrix) bioink and LaminInk + (Cellink) laminin bioink were first transferred to a 5 ml plastic syringe with male-male LuerLock. To reduce the presence of bubbles in the bioink, the loaded syringe was centrifuged for 4 mins at 1200 x g, with the aid of a custom-made centrifuge insert. The hydrogel was next transferred to a 1 ml Hamilton gastight syringe via a female-female LuerLock adapter. The syringe was then inserted into the 3D-printed syringe holder, which in turn was bolted into the syringe pump body with four M3x10 screws.

FRESH collagen bioprinting, cell seeding, and construct imaging

FRESH bioprinting was performed according to the protocol by Lee et al.¹⁶, using LifeInk 240 (Advanced Biomatrix). The FRESH LifeSupport powder (Cellink), from which the gelatin microparticle support bath was prepared, was used as per the manufacturer's instructions. Following print completion, the tool was left at the tool dock and the build plate lowered. All constructs generated using FRESH bioprinting was made in a custom-designed and easily moveable basket. After a completed print, the basket holding the collagen construct was placed at 37°C for 1 h to melt the gelatin support material and to thereby release the printed construct. Constructs were washed three times in 1x phosphate buffered saline (PBS, Gibco) and stored in PBS at 4°C until further use. For fluorescent imaging, collagen constructs were stained for 1 h at 37°C with 10 µM Col-F (ImmunoChemistry Technologies, Bloomington, USA) prepared in 1x PBS, and then washed twice (5 mins each) with 1x PBS at room temperature. Constructs were imaged by confocal microscopy performed on a Zeiss LSM700 (Zeiss, Jena, Germany) instrument and images were captured using Zen software (Zeiss). For cell seeding, FRESH constructs were first typically stored overnight at 4°C in 1x PBS supplemented with the antibiotics penicillin and streptomycin (PenStrep; ThermoFisher, Uppsala, Sweden). Individual constructs were next moved to separate wells in a µ-slide 8-well coverglass-bottomed chamber (Ibidi) and a cell suspension of 30 x 10³ MDA-MB-231 cells diluted in 250 µl culture medium supplemented with 1x PenStrep per well was deposited directly onto the collagen construct or into an adjacent, construct-free wells, and cultured for 20 h under standard cell culture conditions. Cell staining and analysis of viability and cell morphology by microscopy are described below.

Analysis of cell viability in seeded FRESH collagen constructs

To assess cell viability in FRESH bioprinted collagen constructs, cell-seeded constructs were incubated with the NucBlue nuclear stain to detect individual cells (Invitrogen, Thermo Fisher), propidium iodide (PI) to identify dead cells (1:1000; Invitrogen, Thermo Fisher), and the Cell event caspase-3/7 stain that reports on the activity of caspase 3 and 7 in apoptotic cells (10 µM; Cell event, Invitrogen, Thermo Fisher). Staining solutions were diluted in OptiMEM (Gibco, Thermo Fisher), supplemented with 1x PenStrep. To control for the effectiveness of the viability stains, cells were treated for 5 h with staurosporine (10 µM;

Abcam, Cambridge, United Kingdom), a potent protein kinase inhibitor known to induce apoptosis. Fluorescent signals for the respective stains were captured by confocal microscopy with an LSM700 instrument and Zen software (Zeiss). Multiple z-planes were captured for cell-laden constructs, while a single in-focus z-plane was captured for cells attached directly to the glass in construct-free wells. These experiments were conducted in duplicate on three independent occasions. Image analysis was conducted in the Fiji version of ImageJ³². For cell-laden collagen constructs, the z-plane containing the highest number of cells was selected for analysis. Individual cells were identified as regions of interest (ROI) by applying a threshold to the NucBlue signal. The ImageJ particle analysis function was applied to this thresholded image to include particles within a size range of 15 – 600 μm^2 . This range excluded non-specific signals from small debris and very large clusters of cells. However, it included smaller cell clusters that could be delineated as individual cells by applying the automatic watershed function to the thresholded image. This ROI mask of individual cells was then overlaid on the PI and Cell event caspase-3/7 channels and the mean fluorescence was recorded in each ROI for each channel. This data was exported to Excel, and mean intensity per ROI and channel was background adjusted using an average from three ROIs measured in cell-free areas of the collagen construct. Data was statistically analyzed using ordinary one-way ANOVA with Tukey's multiple comparisons in GraphPad Prism (Prism).

Analysis of cell attachment and cell morphology

To visualize cells adhering to FRESH bioprinted collagen constructs the cells were labelled overnight with SiR-actin (500 nM; Spirochrome, Switzerland), which permits fluorescence imaging of the actin cytoskeleton. Samples were washed twice in OptiMEM cell culture medium, which was then exchanged for OptiMEM containing the NucBlue nuclear stain. The cells were imaged as described above by confocal microscopy.

Analysis of cell viability following extrusion of cell-laden laminin bioink

Cell-laden laminin bioink was prepared as follows: 100 μl of cell suspension containing 11×10^6 cells /ml was mixed with 1 ml Laminink + Bioink (Cellink) by passing back and forth between two 1 ml syringes. For control, the cell-laden bioink was directly deposited into wells from the plastic syringe without extrusion through a thin needle or nozzle. The remaining ink was loaded into a 250 μl Hamilton glass syringe and bioprinting performed with either 18 G nozzle or 18 G needle. For crosslinking of all constructs including non-printed controls, the recommended Crosslinking Agent (Cellink) was applied for 3-5 minutes. Subsequently, the constructs were washed once in warm (37°C) DMEM Glutamax, supplemented with 10% FBS and 1x PenStrep, and then cultured overnight in the media in a standard incubator (5% CO₂, 37°C). To perform live/dead staining cells were stained with fluorescein diacetate (Sigma) 8 μg /mL and PI, diluted 1:1000 in DMEM Glutamax, supplemented with 10% FBS and 1x PenStrep for 10 min. Then constructs were washed once with 1x PBS and kept in 1x PBS for imaging. Images were taken using an LSM 700 confocal microscope (Zeiss) and a 10x objective. Experiments were conducted in three independent repetitions with a total number of five printed constructs and three non-printed control hydrogels. For each construct four images were taken of a z-plane with high cell density and used for analysis in ImageJ. In ImageJ both channels were thresholded manually and the automatic watershed function applied. Subsequently, the particle analysis tool was used to count the number of live or dead cells. Using Excel, the percentage of viable cells was

calculated for each image. Data was statistically analyzed using ordinary one-way ANOVA with Tukey's multiple comparisons in GraphPad Prism (Prism).

Multi-material bioprinting with collagen and laminin bioinks

Multi-material constructs were bioprinted using acidified collagen (Advanced Biomatrix) and Laminink+ (Cellink) containing cells as described above. Printing was done directly onto a glass slide, followed by incubation in 50 mM HEPES (pH 7.4) containing 50 mM CaCl₂, to induce gelation of collagen and laminin, respectively.

Data availability

STL and STEP files, slicing profiles, configuration files, macros and a bill of materials are included as Supplementary Information. The datasets generated and analyzed are available on request.

Acknowledgements

This study was funded by grants to J.K. from the Swedish Cancer Society (# 20 1285 PjF) and by Sweden's Innovation Agency VINNOVA, grant number 2019-00029 and by support from Uppsala University. 3D-printing was performed at U-PRINT; Uppsala University's 3D-printing facility at the Disciplinary Domain of Medicine and Pharmacy and SciLifeLab Uppsala.

Author contributions

A.E., C.S., O.E., P.O.C., and J.K. designed the study. A.E. built the bioprinter and A.E and C.S. performed the experiments. A.E., C.S., O.E., P.O.C., and J.K. analyzed the data, A.E., C.S., O.E., P.O.C., and J.K. wrote and approved the submitted paper.

Supplementary information

Supplementary data (a bill of materials, STL and STEP files, slicing profiles, configuration files, and macros) accompany this paper as separate files.

Competing interests

A.E., C.S., O.E., P.O.C., and J.K. declare no competing financial or non-financial interests.

Figure Legends

Figure 1. Overview of the open source bioprinter based on the E3D motion system and tool changer. (a) Front view and side view CAD illustrations of the open source bioprinter. A transparent polycarbonate box with an integrated HEPA filter with an air intake fan encloses the tool changer to reduce the risk for contamination during the bioprinting process. The tool changer, which is translated along the x- and y-axes, and can retrieve tools from four different tool positions (four syringe pump extrusion tools are shown). The print platform is translated along the z-axis and is equipped with a calibration camera with a microswitch that is used to correct for changes in extrusion position following a change of syringe pump tool. A touch screen attached to the exterior of the cabinet facilitates control of tool selection and calibration functions. (b) Isometric views of the open source bioprinter. The left panel presents a photograph of the assembled bioprinter and the right panel presents a CAD illustration.

Figure 2. Design of the syringe pump extrusion tool. (a) A photograph of the assembled syringe pump extrusion tool. The syringe plunger is pushed down by a lead screw via a plunger press. The lead screw is linearly translated along the z-axis through a stepper motor, which is attached atop the 3D printed plunger housing. 3D printed exchangeable syringe mounts are attached to the base of the plunger housing, and the entire syringe pump extrusion tool is attached to the tool exchanger system via the E3D tool mount fixture. (b) Isometric and exploded views of CAD illustrations of the syringe pump extrusion tool.

Figure 3. FRESH bioprinting using the open source bioprinter. (a) Design of the construct to be printed using FRESH methodology, and (b) actual FRESH bioprinted construct. (c) 3D rendering of a Col-F stained bioprinted collagen construct based on imaging by confocal microscopy. (d) Example of MDA-MB-231 breast cancer cells seeded onto a bioprinted collagen construct post printing. The cells were stained with SiR-actin and NucBlue to visualize the actin cytoskeleton and cell nuclei respectively. The cells were shown to attach and adopt normal cell morphologies a few hours after cell seeding. The relative level of active apoptosis (e) as measured by Caspase 3/7 activity, and relative occurrence of dead cells (f) as measured by propidium iodide signal in cells grown in glass-bottomed wells or on FRESH bioprinted collagen constructs, in the presence or absence of the apoptosis-inducing toxin staurosporine (10 µM for 5 h) are shown.

Figure 4. Multi-material bioprinting using the open source bioprinter.

(a) Example of fluorescein diacetate and propidium iodide (live/dead) staining of MDA-MB-231 breast cancer cells extruded in laminin bioink. (b) Analysis of cell viability after mixing with laminin bioink and extruded or not through an 18 G needle or an 18 G nozzle. (c) Design of the multi-material construct to be printed using both collagen (green) and cell-laden laminin (red) bioinks, as viewed from above illustrating the print path. (d) Image of the bioprinted multi-material construct. (e) Col-F staining of the collagen bioink (green) and Celltracker red staining of MDA-MB-231 cells distributed in the laminin bioink.

References

- 1 Griffith, L. G. & Naughton, G. Tissue Engineering--Current Challenges and Expanding Opportunities. *Science* **295**, 1009-1014, doi:10.1126/science.1069210 (2002).
- 2 Langer, R. & Vacanti, J. Tissue engineering. *Science* **260**, 920-926, doi:10.1126/science.8493529 (1993).
- 3 Peng, W. et al. 3D bioprinting for drug discovery and development in pharmaceuticals. *Acta Biomaterialia* **57**, 26-46, doi:<https://doi.org/10.1016/j.actbio.2017.05.025> (2017).
- 4 Satpathy, A. et al. Developments with 3D bioprinting for novel drug discovery. *Expert Opin Drug Discov* **13**, 1115-1129, doi:10.1080/17460441.2018.1542427 (2018).
- 5 Humphreys, B. D. Bioprinting better kidney organoids. *Nature Materials* **20**, 128-130, doi:10.1038/s41563-020-00881-5 (2021).
- 6 Kang, H.-W. et al. A 3D bioprinting system to produce human-scale tissue constructs with structural integrity. *Nature Biotechnology* **34**, 312-319, doi:10.1038/nbt.3413 (2016).
- 7 Murphy, S. V. & Atala, A. 3D bioprinting of tissues and organs. *Nature Biotechnology* **32**, 773-785, doi:10.1038/nbt.2958 (2014).
- 8 Jovic, T. H., Combellack, E. J., Jessop, Z. M. & Whitaker, I. S. 3D Bioprinting and the Future of Surgery. *Front Surg* **7**, 609836-609836, doi:10.3389/fsurg.2020.609836 (2020).

- 9 Ong, C. S. *et al.* 3D bioprinting using stem cells. *Pediatr Res* **83**, 223-231, doi:10.1038/pr.2017.252 (2018).
- 10 Ozbolat, I. T. & Hospoduk, M. Current advances and future perspectives in extrusion-based bioprinting. *Biomaterials* **76**, 321-343, doi:10.1016/j.biomaterials.2015.10.076 (2016).
- 11 Li, J., Chen, M., Fan, X. & Zhou, H. Recent advances in bioprinting techniques: approaches, applications and future prospects. *Journal of Translational Medicine* **14**, 271, doi:10.1186/s12967-016-1028-0 (2016).
- 12 Boularaoui, S., Al Hussein, G., Khan, K. A., Christoforou, N. & Stefanini, C. An overview of extrusion-based bioprinting with a focus on induced shear stress and its effect on cell viability. *Bioprinting* **20**, e00093, doi:<https://doi.org/10.1016/j.bprint.2020.e00093> (2020).
- 13 Fitzsimmons, R. E. B. *et al.* Generating vascular channels within hydrogel constructs using an economical open-source 3D bioprinter and thermoreversible gels. *Bioprinting* **9**, 7-18, doi:<https://doi.org/10.1016/j.bprint.2018.02.001> (2018).
- 14 Thomas, A. *et al.* Vascular bioprinting with enzymatically degradable bioinks via multi-material projection-based stereolithography. *Acta Biomaterialia* **117**, 121-132, doi:<https://doi.org/10.1016/j.actbio.2020.09.033> (2020).
- 15 Hinton, T. J. *et al.* Three-dimensional printing of complex biological structures by freeform reversible embedding of suspended hydrogels. *Sci Adv* **1**, e1500758, doi:10.1126/sciadv.1500758 (2015).
- 16 Lee, A. *et al.* 3D bioprinting of collagen to rebuild components of the human heart. *Science* **365**, 482-487, doi:10.1126/science.aav9051 (2019).
- 17 Shiawski, D. J., Hudson, A. R., Tashman, J. W. & Feinberg, A. W. Emergence of FRESH 3D printing as a platform for advanced tissue biofabrication. *APL Bioeng* **5**, 010904-010904, doi:10.1063/5.0032777 (2021).
- 18 Kahl, M., Gertig, M., Hoyer, P., Friedrich, O. & Gilbert, D. F. Ultra-Low-Cost 3D Bioprinting: Modification and Application of an Off-the-Shelf Desktop 3D-Printer for Biofabrication. *Frontiers in Bioengineering and Biotechnology* **7**, doi:10.3389/fbioe.2019.00184 (2019).
- 19 Krige, A., Haluška, J., Rova, U. & Christakopoulos, P. Design and implementation of a low cost bio-printer modification, allowing for switching between plastic and gel extrusion. *HardwareX* **9**, e00186, doi:<https://doi.org/10.1016/j.ohx.2021.e00186> (2021).
- 20 E3D-Online, E. s. f. D. p. *E3D-Online, Extrusion systems for 3D printing*, <<https://e3d-online.com/pages/about>> (2021).
- 21 files_GitHub, E. D.-o. T. *E3D-online ToolChanger files_GitHub*, <<https://github.com/e3donline/ToolChanger>> (
- 22 Pusch, K., Hinton, T. J. & Feinberg, A. W. Large volume syringe pump extruder for desktop 3D printers. *HardwareX* **3**, 49-61, doi:<https://doi.org/10.1016/j.ohx.2018.02.001> (2018).
- 23 Tashman, J. W., Shiawski, D. J. & Feinberg, A. W. A high performance open-source syringe extruder optimized for extrusion and retraction during FRESH 3D bioprinting. *HardwareX* **9**, e00170, doi:<https://doi.org/10.1016/j.ohx.2020.e00170> (2021).
- 24 Kolesky, D. B., Homan, K. A., Skylar-Scott, M. A. & Lewis, J. A. Three-dimensional bioprinting of thick vascularized tissues. *Proceedings of the National Academy of Sciences* **113**, 3179-3184, doi:10.1073/pnas.1521342113 (2016).
- 25 Liu, Y. *et al.* The stiffness of hydrogel-based bioink impacts mesenchymal stem cells differentiation toward sweat glands in 3D-bioprinted matrix. *Materials Science and Engineering: C* **118**, 111387, doi:<https://doi.org/10.1016/j.msec.2020.111387> (2021).
- 26 Ding, H., Illsley, N. P. & Chang, R. C. 3D Bioprinted GelMA Based Models for the Study of Trophoblast Cell Invasion. *Scientific Reports* **9**, 18854, doi:10.1038/s41598-019-55052-7 (2019).
- 27 Freeman, F. E. & Kelly, D. J. Tuning Alginate Bioink Stiffness and Composition for Controlled Growth Factor Delivery and to Spatially Direct MSC Fate within Bioprinted Tissues. *Scientific Reports* **7**, 17042, doi:10.1038/s41598-017-17286-1 (2017).

- 28 Hamid, O. A., Eltaher, H. M., Sottile, V. & Yang, J. 3D bioprinting of a stem cell-laden, multi-material tubular composite: An approach for spinal cord repair. *Materials Science and Engineering: C* **120**, 111707, doi:<https://doi.org/10.1016/j.msec.2020.111707> (2021).
- 29 Mehesz, A. N. *et al.* Scalable robotic biofabrication of tissue spheroids. *Biofabrication* **3**, 025002, doi:10.1088/1758-5082/3/2/025002 (2011).
- 30 Moldovan, N. I., Hibino, N. & Nakayama, K. Principles of the Kenzan Method for Robotic Cell Spheroid-Based Three-Dimensional Bioprinting<sup>. *Tissue Eng Part B Rev* **23**, 237-244, doi:10.1089/ten.TEB.2016.0322 (2017).
- 31 Li, N. T. *et al.* Development of a bioprinting approach for automated manufacturing of multi-cell type biocomposite TRACER strips using contact capillary-wicking. *Biofabrication* **12**, 015001, doi:10.1088/1758-5090/ab47e8 (2019).
- 32 Schindelin, J. *et al.* Fiji: an open-source platform for biological-image analysis. *Nature Methods* **9**, 676-682, doi:10.1038/nmeth.2019 (2012).

Figure 1

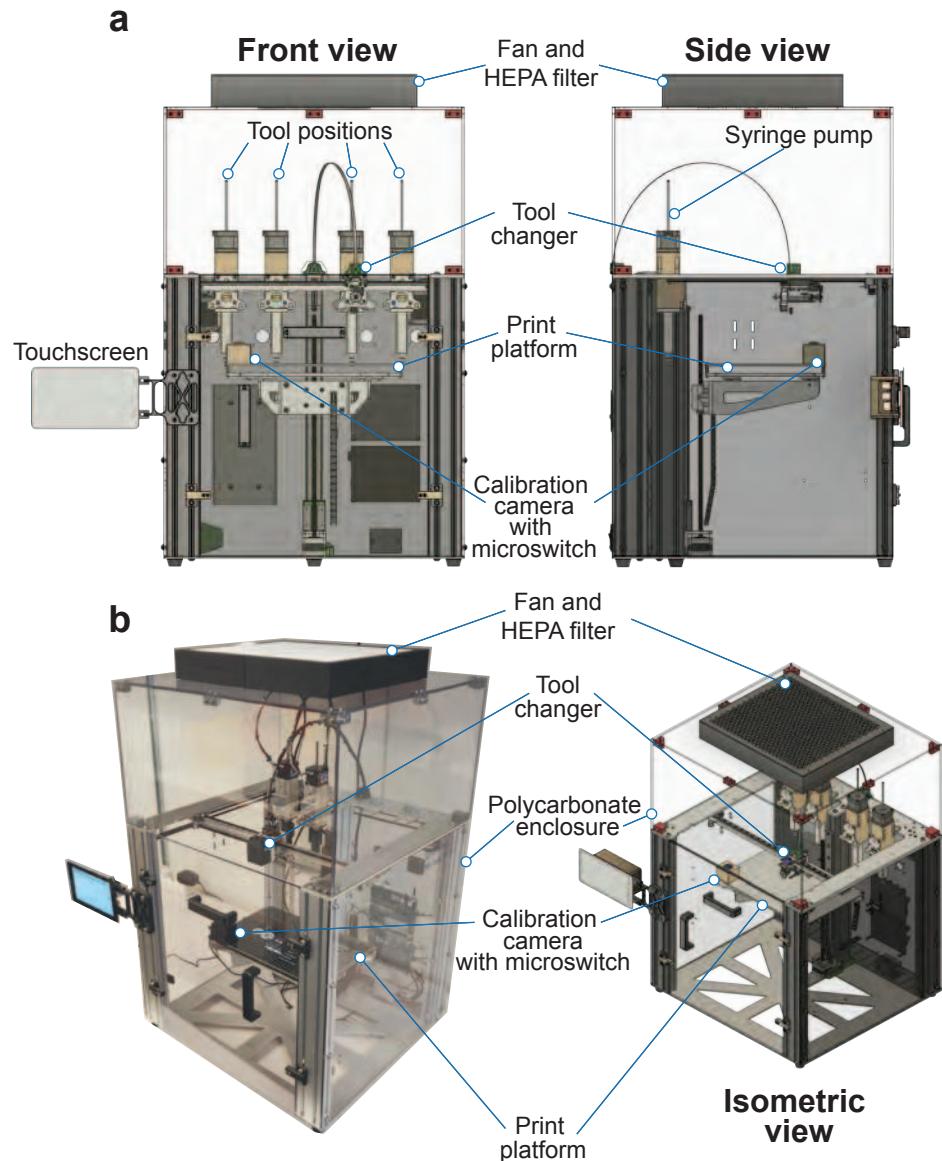


Figure 2

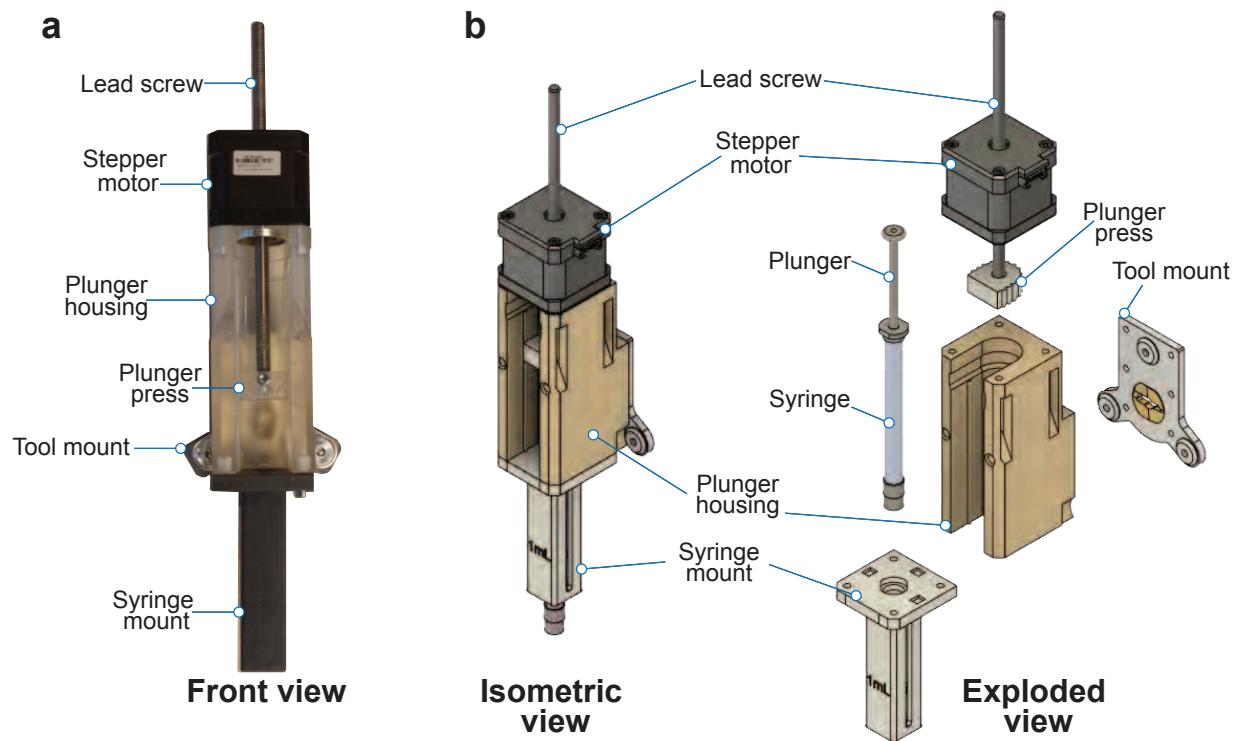


Figure 3


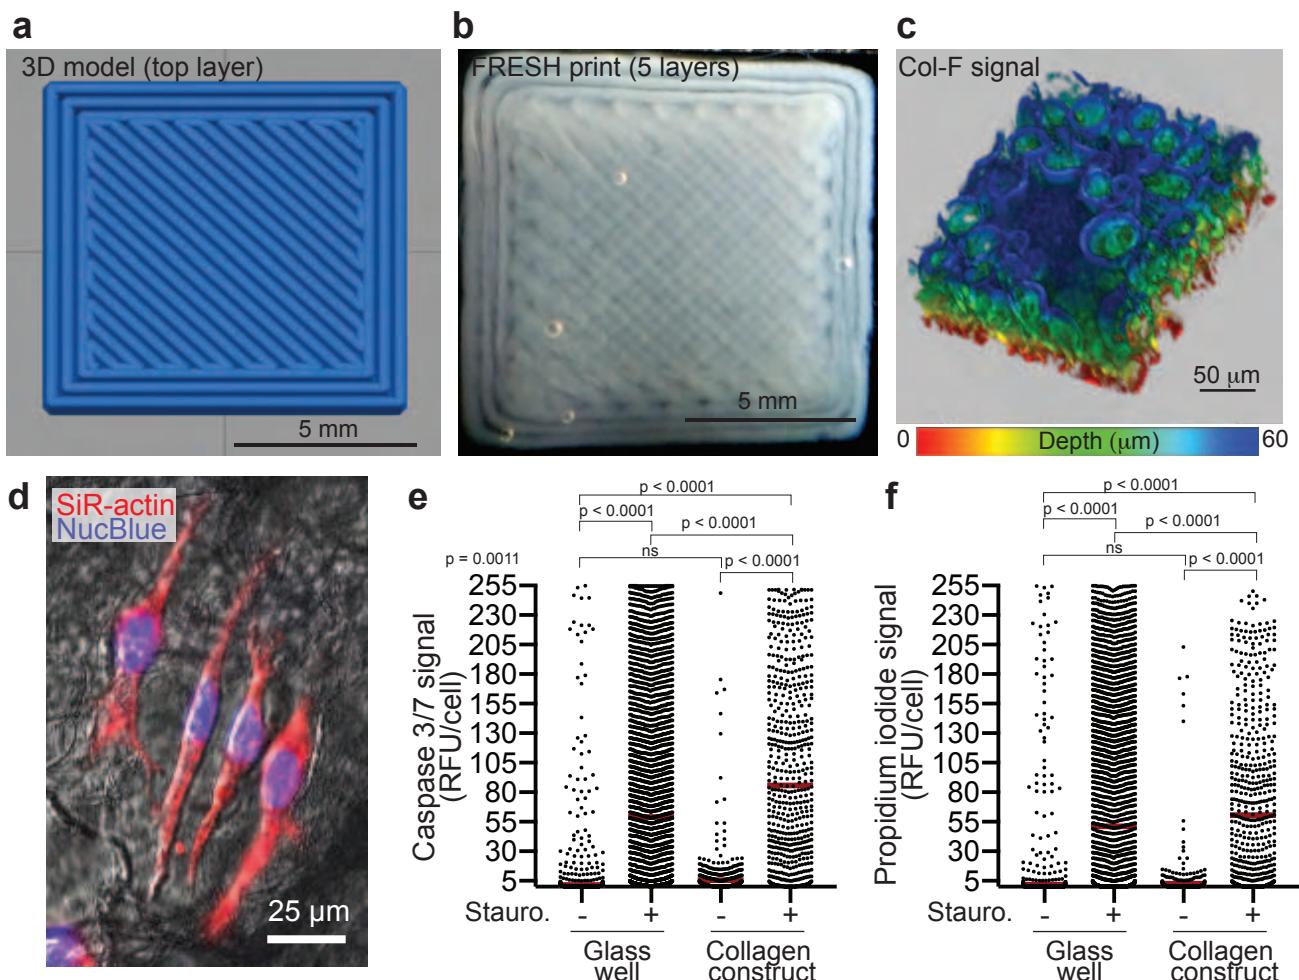


Figure 4

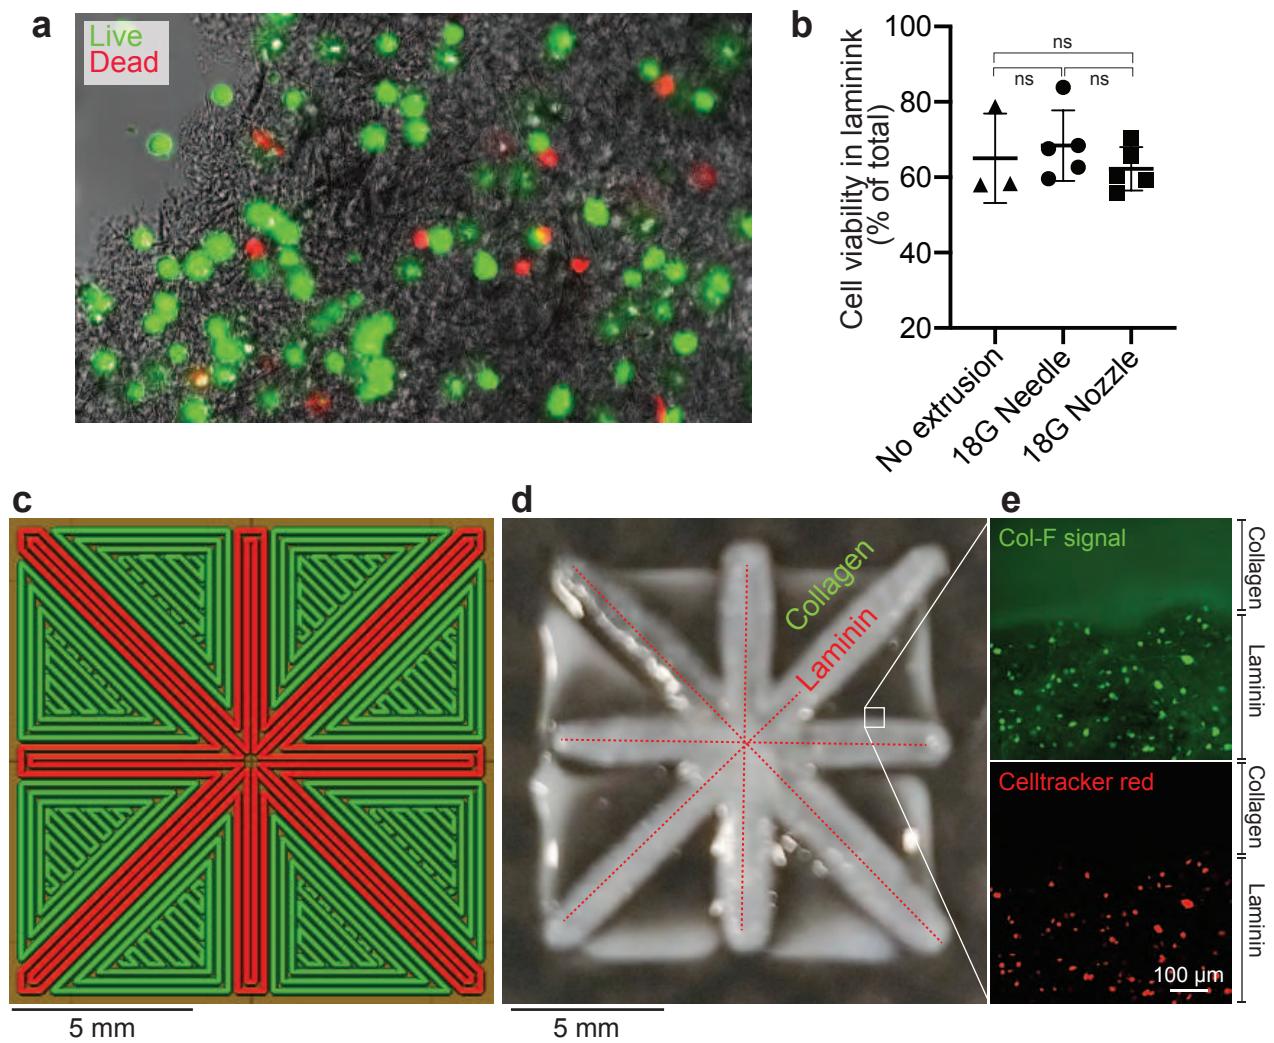

Supplementary Files

This is a list of supplementary files associated with this preprint. Click to download.

- [Billofmaterials.xlsx](#)
- [PrintercomponentsSTLandSTEPfiles.zip](#)
- [Slicingprofilesconfigurationfilesandmacros.zip](#)
- [Supplementaryinformationindex.docx](#)