

Comparison of the Agatston score acquired with photon-counting detector CT and energy-integrating detector CT: *Ex vivo* study of cadaveric hearts

Susann Skoog (✉ Susann.Skoog@regionostergotland.se)

Linkoping University Faculty of Medicine: Linkopings universitet Medicinska Fakulteten <https://orcid.org/0000-0001-5309-0829>

Lilian Henriksson

Linkoping universitet medicinska fakulteten

Håkan Gustafsson

department of Medical Radiation Physics

Mårten Sandstedt

Linkoping University Faculty of Medicine: Linkopings universitet Medicinska Fakulteten

Sebastian Elvelind

Linkoping University Faculty of Medicine: Linkopings universitet Medicinska Fakulteten

Anders Persson

Linkoping University Faculty of Medicine: Linkopings universitet Medicinska Fakulteten

Research Article

Keywords: Photon counting detector CT, CT-angiography, heart, arteriosclerosis, Calcium, Coronary vessels

Posted Date: October 18th, 2021

DOI: <https://doi.org/10.21203/rs.3.rs-973623/v1>

License:  This work is licensed under a Creative Commons Attribution 4.0 International License. [Read Full License](#)

Version of Record: A version of this preprint was published at The International Journal of Cardiovascular Imaging on January 5th, 2022. See the published version at <https://doi.org/10.1007/s10554-021-02494-8>.

Abstract

The purpose of this study was to compare the correlation and agreement between AS derived from either an energy-integrating detector CT (EID-CT) or a photon-counting detector CT (PCD-CT). Reproducibility was also compared.

Method

In total, 26 calcified coronary lesions (from five cadaveric hearts) were identified for inclusion. The hearts were positioned in a chest phantom and scanned in both an EID-CT and a prototype PCD-CT. The EID-CT and PCD-CT acquisition and reconstruction parameters were matched. To evaluate the reproducibility, the phantom was manually repositioned, and an additional scan was performed using both methods. The EID-CT reconstructions were performed using the dedicated calcium score kernel Sa36. The PCD-CT reconstructions were performed with a vendor-recommended kernel (Qr36). Several monoenergetic energy levels (50–150 keV) were evaluated to find the closest match with the EID-CT scans. A semi-automatic evaluation of calcium score was performed on a post-processing multimodality workplace.

Results

The best match with Sa36 was PCD-CT Qr36 images, at a monoenergetic level of 72 keV. Statistical analyses showed excellent correlation and agreement. The correlation and agreement with regards to the Agatston score (AS) between the two methods, for each position as well as between the two positions for each method, were assessed with the Spearman's rank correlation. The correlation coefficient, rho, was 0.98 and 0.97 respectively 0.99 and 0.98. The corresponding agreements were investigated by means of Bland-Altman plots.

Conclusion

High correlation and agreement was observed between the AS derived from the EID-CT and a PCD-CT. Both methods also demonstrated excellent reproducibility.

Introduction

Energy-integrating detector computed tomography (EID-CT) is used for detection of atherosclerotic disease [1–3]. Photon counting detector CT (PCD-CT) technology has recently been introduced [4,5], with expectation for improved clinical applications [6–9]. While EID-CTs convert incoming photons into electric currents using scintillator and photodiode layers indirectly, PCD-CTs directly convert x-ray photons into proportional electric signals using semiconductor materials. These technical characteristics of PCDs offer various advantages over conventional EID technology. Higher spatial resolution can thereby be achieved due to smaller PCD detector pixels. With the PCD technology, low-weighting of low-energy photons leads to better image contrast. This new technology, along with techniques for rendering energy-resolved data, reduces electronic noise resulting in higher dose efficiency, especially in low dose examinations. The reduced level of electronic noise not only results in less image noise but also to fewer streak artifacts and more stable Hounsfield units (HU) numbers [4,5,10,11]. More energy thresholds can be applied, making advanced material decomposition possible [4]. This is a feature expected to have large clinical benefits in coronary CT angiography imaging and characterization of atherosclerotic plaques [15,19].

In clinical practice, coronary calcifications are identified by using Agatston score (AS) evaluations [2,12–15]. AS has shown a high negative predictive value, as an AS of 0 strongly correlates with a lack of cardiovascular events over the following 5 years [15,16]. A disadvantage of the AS is the standardized 3 mm slice thickness, leading to partial volume averaging and calcium blooming artifacts (CBA) [4,17] which may make calcifications appear larger than their true size [14]. Also, partial volume averaging may lead to an underestimation or complete neglect of smaller and less dense calcifications. The result of these misrepresentations has been shown to lead to significant intra- and inter-scan variability for the AS [5,10,12,13].

The consequence of partial volume averaging may be false negative AS of smaller and less dense calcifications. Patients with low calcium score are at higher risk compared to those with zero calcium, and medical therapy might be considered

[14,18,19].

In a study using an anthropomorphic phantom, Van der Werf et al. reported comparable CAC scores for routine clinical protocols between conventional CTs and PCD-CTs. Furthermore, they showed PCD-CT to have increased detectability and accuracy in CAC volume estimation at reduced slice thickness [20]. Symoms et al.'s study demonstrated the potential of PCD technology to improve CAC score image quality and/or reduced radiation dose while maintaining diagnostic image quality. Their study was performed with a cardiac CT phantom, *ex vivo* hearts and asymptomatic volunteers [21]. Both studies were performed with a lower and a higher threshold setting in the PCD-CT and not with different monoenergy levels. Eberhard et al investigated CAC score in PCD-CT compared to EID-CT with different doses of radiation, different QIR and different monoenergy levels. The study showed decreasing CAC scores at increasing QIR levels and increasing keV levels [21].

The purpose of our study was to compare the correlation and agreement between the AS derived from an EID-CT and a PCD-CT. Reproducibility was also compared.

Material And Methods

Ethics

The study was approved by the Swedish Ethical Review Authority (Dnr 2020-06114.).

EID-CT and PCD-CT image acquisition and reconstructions

Five cadaveric hearts were positioned in a chest phantom (N1 Lungman; Kyoto Kagaku Co. Ltd, Japan) and scanned in both an EID-CT (SOMATOM Force; Siemens Healthineers, Forchheim, Germany) as well as in a PCD-CT prototype (SOMATOM Count Plus; Siemens Healthineers, Forchheim Germany).

ECG-gating was not available in the PCD-CT. The vendor-provided spiral cardiac CAC Score protocol on the EID-CT is ECG-gated and ECG dose modulated. Thus, the expressed CTDI_{vol} is based on the average tube current of the whole scan including both low and full dose cardiac phases. As only the full dose phases were used for image reconstructions, the expressed CTDI_{vol} on the EID-CT, would render a too low radiation output on the PCD-CT. In order to get non-gated spiral protocols with an equal radiation output on both systems, we therefore performed the following procedure on the chest phantom before the first examination:

1. A CAC Score ECG-gated spiral scan of the phantom was made using a synthetic ECG on the EID-CT. Automatic exposure control (CARE Dose4D, Siemens Healthineers), vendor recommended Q. ref. mAs of 80 and ECG dose modulation was used. Image reconstructions were made during the full dose phase at 70% of the cardiac cycle using a 160 mm FoV. The dedicated Calcium Score kernel Sa36, as well as a 3 mm slice thickness with 1.5 mm increment were applied, as recommended by the vendor.
2. In total, nine non-ECG-gated spiral test scans were made on the EID-CT with automatic mAs exposure control (CARE Dose4D, Siemens Healthineers) using different Q. ref. mAs settings between 10 and 50. All scans were reconstructed in the same manner as the ECG-gated spiral.
3. The noise level in each test scan was determined by the placement of equal sized regions of interest (ROI) in the slices with the same slice position and at the same location in the image. By comparing the standard deviation (SD) in the non-ECG-gated scans with the SD in the ECG-gated scan a suitable Q. ref. mAs setting was found, i.e. the one rendering equal image noise (35 mAs). This Q. ref. mAs setting was then applied in the non-ECG-triggered thorax protocol used for all the following cadaveric heart scans at the EID-CT within the study.

Scans of the cadaveric hearts at the PCD-CT were made directly after the scans on the EID-CT. By matching the CTDI_{vol} between the scans as closely as possible (CTDI_{vol} varying between 0.85 and 1.14 mGy between the different

cadaveric hearts) a similar radiation output was ensured. All scans within the study were performed with a spiral protocol, using a tube potential of 120 kV. In order to evaluate the reproducibility on both systems, the phantom was scanned once and then manually repositioned, after which it was scanned again.

Reconstructions were performed using quantitative kernels for calcium scoring, i.e. Sa36 for the EID-CT data and Qr36 kernel for the PCD-CT data. Images from both systems were reconstructed with a slice thickness of 3 mm and an increment of 1.5 mm. Details on the acquisition and reconstruction parameters are summarized in Table 1.

Table 1. CT acquisition and reconstruction parameters for energy-integrating detector CT (EID-CT) and photon counting detector CT (PCD-CT) scans.

	EID-CT	PCD-CT
CT acquisition and reconstruction parameters	(SOMATOM Force; Siemens Healthineers)	(SOMATOM Count Plus; Siemens Healthineers).
Scan mode	Non-gated Spiral	Non-gated Spiral
CTDIvol (mGy)	0.88 to 1.14	0.92 to 1.12
Tube potential (kV)	120	120
Pitch	1.2	1.2
Collimation (mm)	192x0.6	144x0.4
Rotation time (s)	0.25	0.33
Monoenergetic levels (keV)		50, 65, 68, 70, 72, 150
Reconstruction technique	WFBP (standard)	IR1 (WFBP was not selectable)
Kernel	Sa36	Qr36
Slice thickness (mm)	3	3
Increment (mm)	1.5	1.5
Reconstruction field of view (mm)	160	160
Image matrix size	512	512

Coronary calcification inclusions

A total of 26 well-defined calcified coronary calcifications with volumes between 1 and 210 mm³ were identified and included in the study. Four to eight calcifications per heart were analysed. The calcifications were located in the left anterior descending artery circumflex artery and/or the right coronary artery

Determination and comparison of AS

The image analyses were performed by a thoracic radiologist with twenty years of radiologic experience, and approximately ten years of experience in cardiac imaging.

Evaluations of the AS were performed using the semi-automatic calcium score analysis software on a post-processing multimodality workplace (Leonardo MMWP, Siemens, Germany).

The AS values of all the included 26 calcifications were compared between the Sa36 reconstructions from the EID-CT and the monoenergetic Qr36 reconstructions from the PCD-CT. The monoenergetic levels available ranged between 50 keV and 150 keV.

Image noise measurements

Image noise was defined as the SD of the mean HU value in a 1 cm² ROI, measured in soft tissue/myocardium in the cadaveric hearts. Two ROIs were placed in each cadaveric heart in both positions in Sa36 (EID-CT) and Qr36, energy level 72 keV (PCD-CT).

Statistics

Continuous data are presented as mean +/- SD if normally distributed, or as median and interquartile range (IQR) if non-normally distributed. The normality assumption was checked visually using p-p-plots.

The correlation and agreement with regard to the AS, both between the two methods for each position, and between the two positions for each method, were assessed with Spearman's rank correlation coefficient, as appropriate for non-parametric data. The agreement was investigated by means of Bland-Altman plots. Although the measurements in themselves were not normally distributed, visual assessments of p-p plots found the normality assumptions for Bland-Altman plots (differences) to hold. Statistical analyses were performed using SPSS Statistics 27 (IBM, Armonk, New York). P-values below 0.05 were considered statistically significant.

Results

The best possible match for, Sa36 in the EID-CT images was Qr36, at a monoenergetic level of 72 keV in the PCD-CT images. (Table 2. For all lesions see appendix)

Table 2. Medians in EID-CT (Sa36) in respect to different monoenergy levels in PCD-CT in positions 1(a) and 2(b).

Table 2a. position 1

	Sa36	Qr36mono50	Qr36mono65	Qr36mono68	Qr36mono70	Qr36mono72	Qr36mono150
N	26	26	26	26	26	26	26
25 th percentile	6.800	29.200	15.325	10.800	9.525	8.950	0.100
50 th percentile (median)	19.500	54.600	30.550	23.900	23.450	22.550	4.100
75 th percentile	38.500	116.075	56.225	53.425	50.750	49.700	11.325

Table 2b. position 2 text text text.

	Sa36	Qr36mono50	Qr36mono65	Qr36mono68	Qr36mono70	Qr36mono72	Qr36mono150
N	26	26	26	26	26	26	26
25 th percentile	7.800	31.150	14.250	11.925	10.575	11.025	0.300
50 th percentile (median)	18.850	54.300	33.200	25.000	22.950	21.500	2.950
75 th percentile	35.750	109.125	64.525	52.050	59.725	48.325	14.025

The correlation between the PCD-CT and EID-CT for position one and two with regards to the AS was analysed with Spearman's rank correlation coefficient and showed $\rho=0.98$ and 0.97 , respectively ($p<0.001$) (Figure 1). The Bland Altman mean difference and 1.96 standard deviations (SD) upper and lower limits of agreements for the AS between the EID-CT and PCD-CT were -5.43 (7.2 to -18.1) and -6.39 (9.5 to -22.3) for position one and two, respectively, (Figure 2).

The correlation between position one and two for the EID-CT and PCD-CT with regards to the AS was (ρ) =0.99 and 0.98 ($p<0.001$) respectively (Figure 3). The Bland Altman mean difference and 1.96 SD upper and lower limits of agreements for the AS between position one and two were 1.26 (7.7 to -5.2) for the EID-CT and 0.14 (8.4 to -8.1) for the PCD-CT, respectively. (Figure 4).

The average image noise in the EID-CT Sa36 and the PCD-CT Qr36 monoenergetic (72 keV) was 12.2 (+/-2.1) and 14 (+/-2.1) HU, respectively.

Discussion

In this *ex vivo* study of cadaveric hearts, there was an excellent correlation and agreement between the AS derived from an EID-CT and a PCD-CT. Also, both methods demonstrated an excellent reproducibility.

Measurement of the AS has long been the clinical standard for quantification of coronary calcium and still remains the most commonly used CAC score in clinical practice [13–15]. The PCD-CT is a promising technique on the verge of becoming clinically feasible. When introducing a new technique for clinical examination, it is important to determine if well-established scoring methods, such as the AS, remain reliable for early detection and risk stratification of CAD.

The augmented PCD-CT detector technology, counting every incoming photon, resulted in a slight AS overestimation tendency according to the Bland Altman analysis. In PCD-CT, calcification attenuation values acquired at 120 kV are higher than those measured in EID-CT scans. This is due to improved weighting of low-energy photons. To adjust for this as much as possible, monoenergetic images reconstructed at the keV level rendering similar HU values as those in 120 kV images should be used. We investigated the vendor-provided monoenergetic levels at 50, 65, 68, 70, 72 and 150 keV. The best possible match turned out to be reconstructions at 72 keV. If further keV levels were added in the gap between 72 and 150 keV, the slight tendency toward overestimation using the PCD-CT may potentially be compensated for, likely resulting in further improved correlation.

The historical tie between the AS and 3 mm slices, limited the improvements possible with the spatial resolution provided by the PCD-CT technique in this study.

Both the EID-CT and the PCD-CT exhibited good reproducibility which, at least to some extent, may be explained by the average noise being similar between the methods.

PCD-CT technology may have additional benefits for CAC scoring, which were beyond the scope of this study. For instance, improved quantification of low or intermediate CAC scores and better evaluation of the distribution and shape of calcifications. This could lead to the method having an even higher prognostic value and better reproducibility than the current AS[5,20,23]. In addition, the improved HU stability, and the lower degree of electronic noise of PCD-CT, may lead to a more reliable CAC score at a lower radiation dose and detection of smaller calcified coronary lesions [21]. Further studies evaluating the possibilities for improved segmentation and quantification of coronary calcifications with the thinner slice thickness possible with PCD technology would be of interest.

The data in our study correspond with results in prior studies aiming to compare CAC scoring in PCD-CT to EID-CT for clinical routine protocols. N. Werf et al. also showed PCD-CT to be superior for detection of CAC at reduced slice thickness which provided more accurate volume scores [20]. R. Symoms et al.'s study demonstrated the potential of PCD technology to improve CAC score image quality and/or reduce radiation dose while maintaining diagnostic image quality[22]. Eberhard et al.'s work suggested accurate CAC scoring using monoenergetic reconstructions, as well as decrease CAC score with increasing strength levels of QIR and increasing monoenergetic levels. [21]

There are some limitations in our study. Results have been generated with a PCD-CT prototype scanner not yet approved for routine clinical use, without availability of any ECG-gated scan protocols. We thereby used non-gated spiral protocols in the PCD-CT as well as in the EID-CT. This led to limited post-processing possibilities as clinical workstations are incompatible with non-ECG triggered CAC scans. Another limitation caused by the post-processing restrictions was, as mentioned above, predetermined keV levels.

Since the study used *ex vivo* cadaveric hearts there was no motion artifacts, as a phantom does not completely simulate an actual human. We used WFBP reconstructions at EID-CT and IR1 at PCD-CT (available IR setting was IR1-5). At the same dose level, we had expected the PCD-CT images to be less noisy than the EID-CT images. There are several potential sources that can cause this rather small difference. For instance, the relatively small ROI, the chosen keV and the difference in data processing. One radiologist performed the image analysis, and no inter-reader analysis was performed. The total AS in each cadaveric heart was not measured, as two of the hearts contained calcifications in other locations such as valves and stents, which were difficult to separate from coronary calcifications.

Conclusion

The study indicates good potential for a conversion of the established Agatston score from EID-CT to the forthcoming PCD-CT technology.

There excellent correlation and agreement was demonstrated between the AS derived from an EID-CT and a PCD-CT. The augmented PCD-CT detector technology, counting every incoming photon, resulted in a slight AS overestimation tendency. Our study showed inter-scan reproducibility to be good both in PCD-CT and EID-CT respectively.

Declarations

Funding: This study has received research funding by ALF grants, Region Östergötland, LIO 899441

Conflicts of interest/Competing interests:

The authors declare that they have no conflict of interest.

The authors of this manuscript declare no relationships with any companies, whose products or services may be related to the subject matter of the article.

Availability of data and material (data transparency)

Data used for this study is available through the corresponding author.

Code availability (software application or custom code)

Not applicable

Authors' contributions (optional: please review the submission guidelines from the journal whether statements are mandatory)

All authors contributed to the study conception and design. Material preparation, data collection and analysis were performed by [Susann Skoog], [Lilian Henriksson] and [Sebastian Elvelind]. The first draft of the manuscript was written by [Susann Skoog] and all authors commented on previous versions of the manuscript. All authors read and approved the final manuscript.

Ethics approval:

Study approved by Swedish Ethical Review Authority (Dnr 2020-06114).

Consent to participate:

Study performed on ex vivo samples. Consent to participate not necessary according to Swedish Ethical Review Authority (Dnr 2020-06114).

Consent for publication (include appropriate statements)

Study performed on ex vivo samples. Consent not necessary for publication according to Swedish Ethical Review Authority (Dnr 2020-06114).

Acknowledgement:

The authors are grateful to Anna Axmon, docent, Division of Occupational and Environmental Medicine, Lund University, who provided help with the statistics.

We are also grateful for the support from Siemens Healthineers regarding the use of the research prototype PCD-CT.

Funding: This study has received research funding by ALF grants, Region Ostergotland, LIO 899441

References

1. Schmermund A, Schwartz RS, Adamzik M, Sangiorgi G, Pfeifer EA, Rumberger JA, Burke AP, Farb A, Virmani R, Coronary atherosclerosis in unheralded sudden coronary death under age 50: Histo-pathologic comparison with "healthy" subjects dying out of hospital, *Atherosclerosis*. (2001). [https://doi.org/10.1016/S0021-9150\(00\)00598-0](https://doi.org/10.1016/S0021-9150(00)00598-0)
2. Agatston AS, Janowitz WR, Hildner FJ, Zusmer NR, Viamonte M, Detrano R (1990) Quantification of coronary artery calcium using ultrafast computed tomography. *Journal of the American College of Cardiology* 15:827–832. [https://doi.org/10.1016/0735-1097\(90\)90282-T](https://doi.org/10.1016/0735-1097(90)90282-T)
3. Wang Y, Osborne MT, Tung B, Li M, Li Y (2018) Imaging cardiovascular calcification. *Journal of the American Heart Association* 7:1–15. <https://doi.org/10.1161/JAHA.118.008564>
4. Flohr T, Ulzheimer S, Petersilka M, Schmidt B (2020) Basic principles and clinical potential of photon-counting detector CT. *Chinese Journal of Academic Radiology* 3:19–34. <https://doi.org/10.1007/s42058-020-00029-z>
5. Willemink MJ, Persson M, Pourmorteza A, Pelc NJ, Fleischmann D (2018) Photon-counting CT: Technical Principles and Clinical Prospects. *Radiology* 289:293–312. <https://doi.org/10.1148/radiol.2018172656>
6. Leiner T, A New Era in Atherosclerotic Plaque Characterization with Photon-counting CT, *Radiology*. (2021) 210313. <https://doi.org/10.1148/radiol.2021210313>

7. Si-Mohamed SA, Sigovan M, Hsu JC, Tatard-Leitman V, Chalabreysse L, Naha PC, Garrivier T, Dessouky R, Carnaru M, Boussel L, Cormode DP, Douek PC, In Vivo Molecular K-Edge Imaging of Atherosclerotic Plaque Using Photon-counting CT, *Radiology*. (2021) 203968. <https://doi.org/10.1148/radiol.2021203968>
8. Sandstedt M, Marsh J, Rajendran K, Gong H, Tao S, Persson A, Leng S, McCollough C, Improved coronary calcification quantification using photon-counting-detector CT: an ex vivo study in cadaveric specimens, *European Radiology* m (2021) 1–17. <https://doi.org/10.1007/s00330-021-07780-6>
9. Rajendran K, Marsh J, Petersilka M, Henning A, Shanblatt E, Schmidt B, Flohr T, Fletcher J, McCollough C, Leng S, High resolution, full field of view, whole body photon-counting detector CT: system assessment and initial experience, in: H. Bosmans, W. Zhao, L. Yu (Eds.), *Medical Imaging 2021: Physics of Medical Imaging*, SPIE (2021) p. 9. <https://doi.org/10.1117/12.2581944>
10. Leng S, Bruesewitz M, Tao S, Rajendran K, Halaweish AF, Campeau NG, Fletcher JG, McCollough CH (2019) Photon-counting detector CT: System design and clinical applications of an emerging technology. *Radiographics* 39:729–743. <https://doi.org/10.1148/rg.2019180115>
11. von Spiczak J, Mannil M, Peters B, Hickethier T, Baer M, Henning A, Schmidt B, Flohr T, Manka R, Maintz D, Alkadhi H, Photon Counting Computed Tomography with Dedicated Sharp Convolution Kernels: Tapping the Potential of a New Technology for Stent Imaging, *Investigative Radiology*. 53 (2018) 486–494. <https://doi.org/10.1097/RLI.0000000000000485>
12. Rumberger J, Brundage B, Rader D, Kondos G, Electron beam computed tomographic coronary calcium scanning: A review and guidelines for use in asymptomatic persons, *Mayo Clinic Proceedings*. 74 (1999) 243–252. <https://doi.org/10.4065/74.3.243>
13. Alluri K, Joshi PH, Henry TS, Blumenthal RS, Nasir K, Blaha MJ (2015) Scoring of coronary artery calcium scans: History, assumptions, current limitations, and future directions. *Atherosclerosis* 239:109–117. <https://doi.org/10.1016/j.atherosclerosis.2014.12.040>
14. Willemink MJ, van der Werf NR, Nieman K, Greuter MJW, Kowek LM, Fleischmann D (2019) Coronary artery calcium: A technical argument for a new scoring method. *Journal of Cardiovascular Computed Tomography* 13:347–352. <https://doi.org/10.1016/j.jcct.2018.10.014>
15. Sandfort V, Bluemke DA (2017) CT calcium scoring. History, current status and outlook. *Diagnostic Interventional Imaging* 98:3–10. <https://doi.org/10.1016/j.diii.2016.06.007>
16. Detrano R, Guerci AD, Carr JJ, Bild DE, Burke G, Folsom AR, Liu K, Shea S, Szklo M, Bluemke DA, O’Leary DH, Tracy R, Watson K, Wong ND, Kronmal RA (2008) Coronary Calcium as a Predictor of Coronary Events in Four Racial or Ethnic Groups. *New England Journal of Medicine* 358:1336–1345. <https://doi.org/10.1056/nejmoa072100>
17. Kalisz K, Buethe J, Saboo SS, Abbara S, Halliburton S, Rajiah P, Artifacts at cardiac CT: Physics and solutions, *Radiographics*. 36 (2016) 2064–2083. <https://doi.org/10.1148/rg.2016160079>
18. Blaha M, Budoff MJ, Shaw LJ, Khosa F, Rumberger JA, Berman D, Callister T, Raggi P, Blumenthal RS, Nasir K, Absence of Coronary Artery Calcification and All-Cause Mortality, *JACC: Cardiovascular Imaging*. 2 (2009) 692–700. <https://doi.org/10.1016/j.jcmg.2009.03.009>
19. Rajan T, Rozanski A, Cainzos-Achirica M, Grandhi GR, Dardari ZA, Al-Mallah MH, Blankstein R, Miedema MD, Shaw LJ, Rumberger JA, Budoff MJ, Blaha MJ, Berman D, Nasir K (2020) Relation of Absence of Coronary Artery Calcium to Cardiovascular Disease Mortality Risk Among Individuals Meeting Criteria for Statin Therapy According to the 2018/2019 ACC/AHA Guidelines, in: *American Journal of Cardiology*. Elsevier Inc., pp 49–55. <https://doi.org/10.1016/j.amjcard.2020.08.050>
20. van der Werf NR, Rodesch PA, van Hamersveld RW, Greuter MJW, Coronary calcium scoring potential of large field-of-view spectral photon-counting CT: a phantom study, (2021)
21. Eberhard M, Mergen V, Higashigaito K, Allmendinger T, Manka R, Flohr T, Schmidt B, Euler A, Alkadhi H, Coronary Calcium Scoring with First Generation Dual-Source Photon-Counting CT—First Evidence from Phantom and In-Vivo Scans,

22. Symons R, Sandfort V, Mallek M, Ulzheimer S, Pourmorteza A (2019) Coronary artery calcium scoring with photon-counting CT: first *in vivo* human experience. International Journal of Cardiovascular Imaging 35:733–739. <https://doi.org/10.1007/s10554-018-1499-6>
23. Mori H, Torii S, Kutyna M, Sakamoto A, Finn Av, Virmani R, Coronary Artery Calcification and its Progression: What Does it Really Mean?, JACC: Cardiovascular Imaging. 11 (2018) 127–142. <https://doi.org/10.1016/j.jcmg.2017.10.012>

Figures

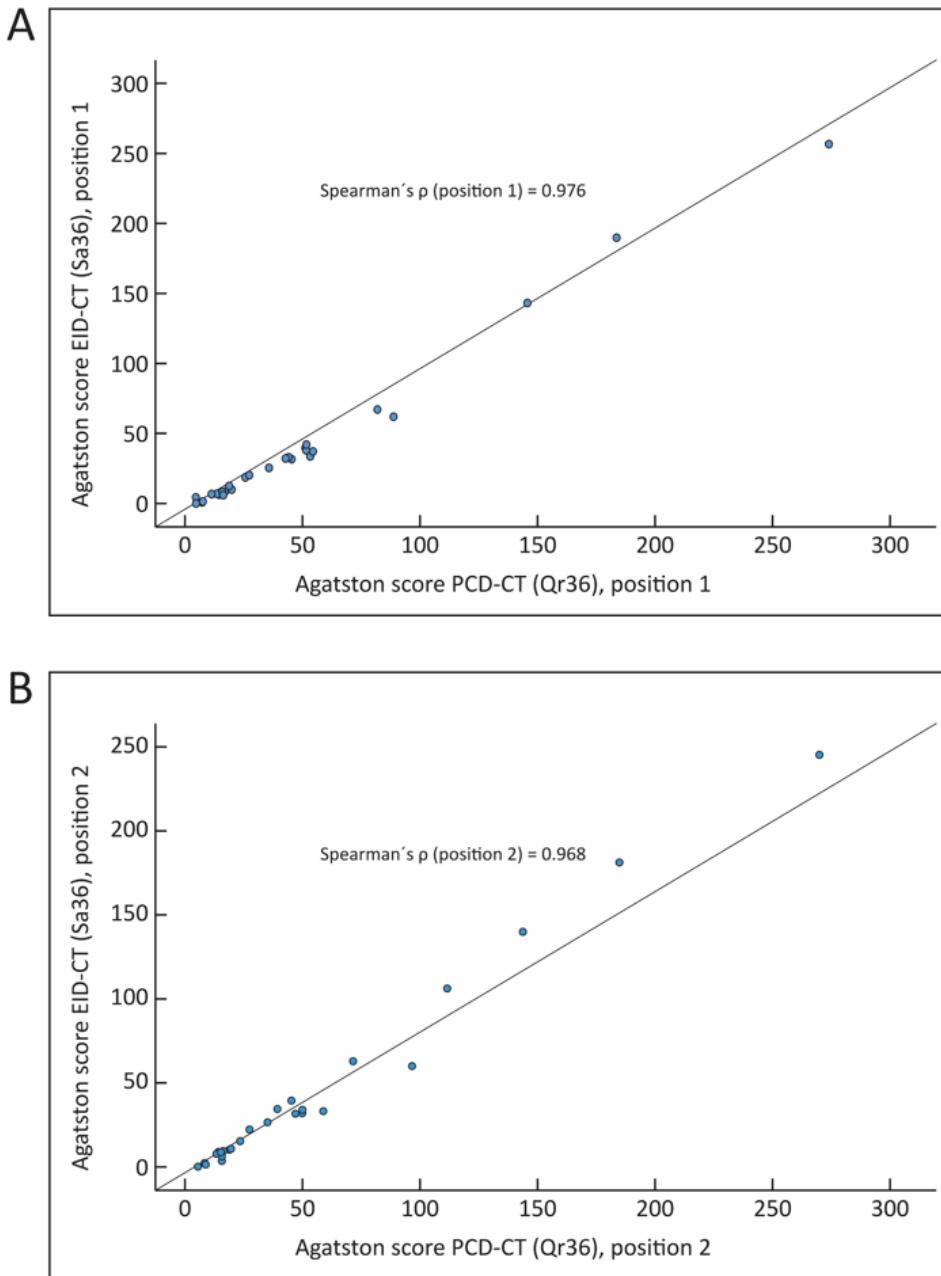


Figure 1

Scatter plot depicting the Agatston score correlation between the EID-CT and PCD-CT, expressed as Spearman rank correlation coefficient (ρ). A) Position one: $\rho = 0.976$. B) Position two: $\rho = 0.968$

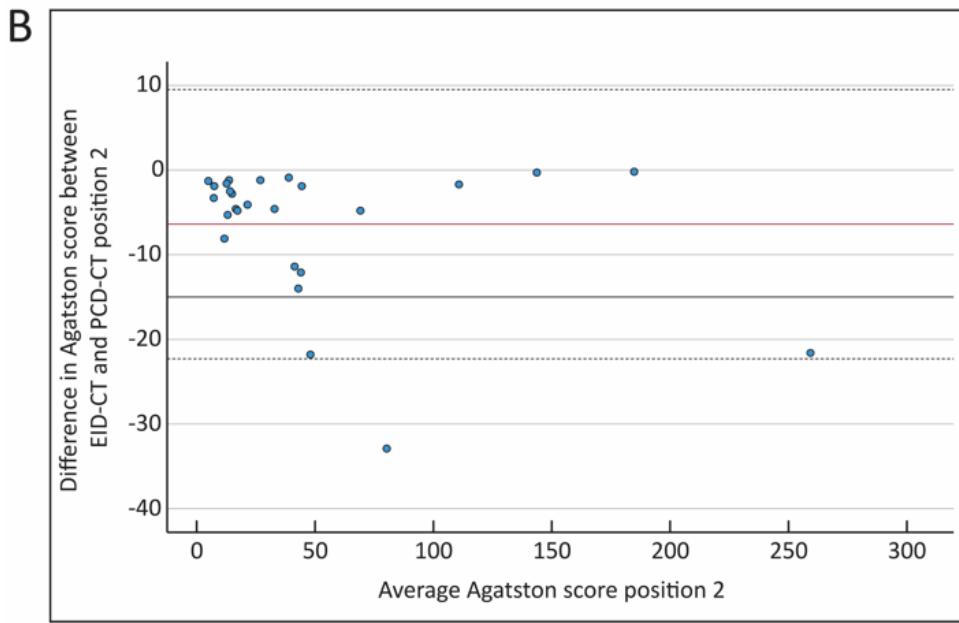
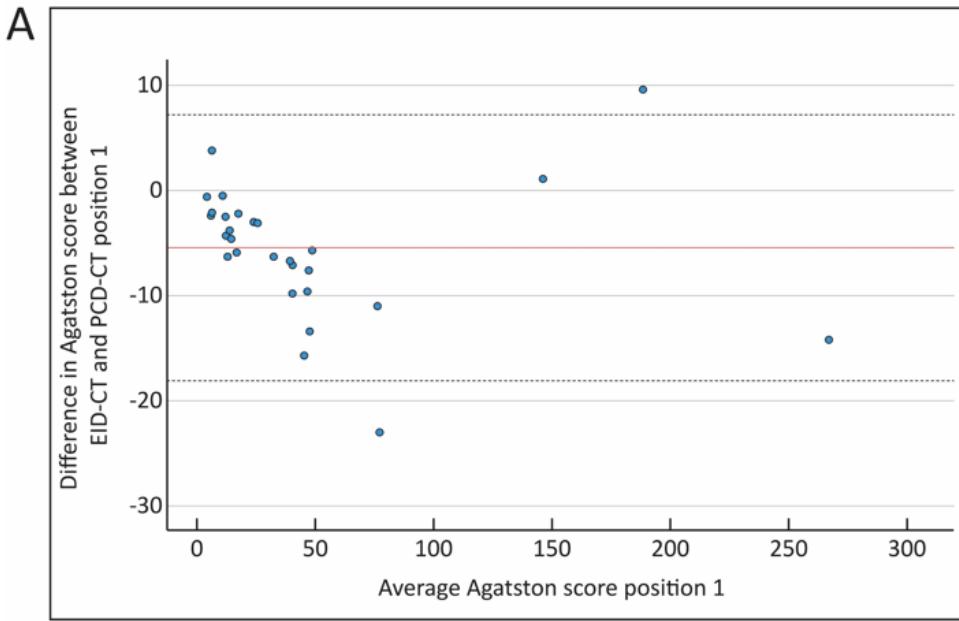


Figure 2

Bland-Altman plot for position 1 (A). The solid red line shows the mean difference between the energy integrating detector CT (EID-CT) and the Photon counting detector CT (PCD-CT) (-5.43). Dashed lines indicate +/- 2 SD (7.2 to -18.1). Bland-Altman plot for position 2 (B). The solid red line shows mean difference between the EID-CT and the PCD-CT (-6.39). Dashed lines indicate +/- 2 SD (9.5 to -22.3)

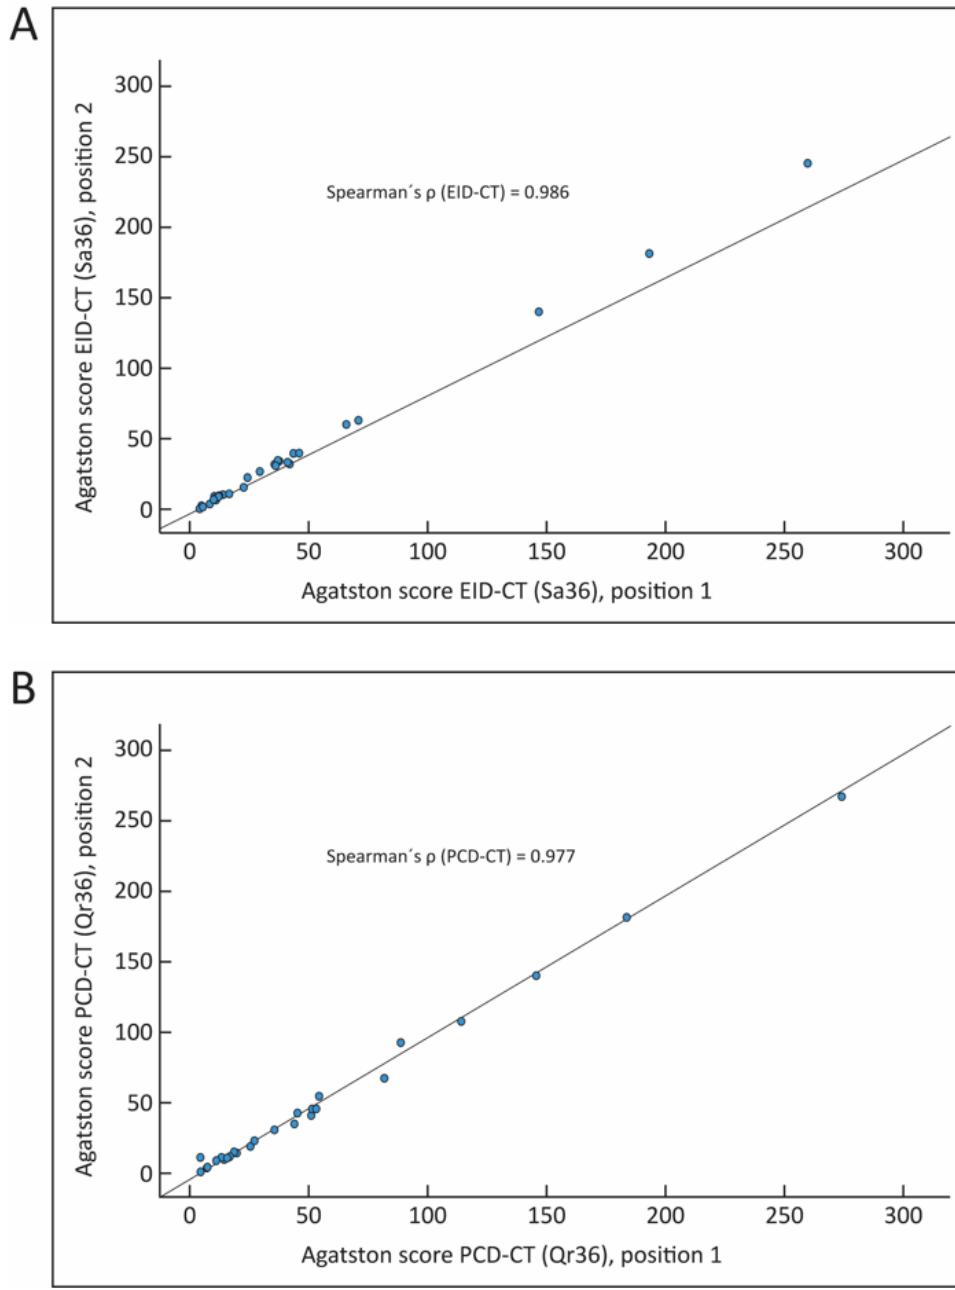


Figure 3

Scatter plot depicting the Agatston score correlation between position one and two in the EID-CT and PCD-CT, expressed as Spearman rank correlation coefficient (ρ). A) EID-CT: $\rho = 0.986$. B) PCD-CT: $\rho = 0.977$

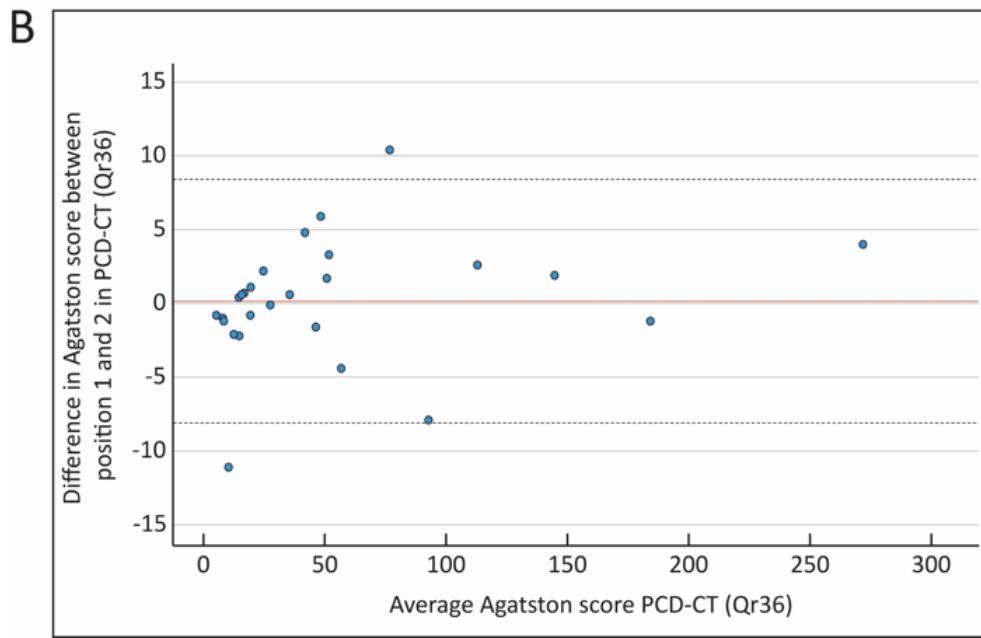
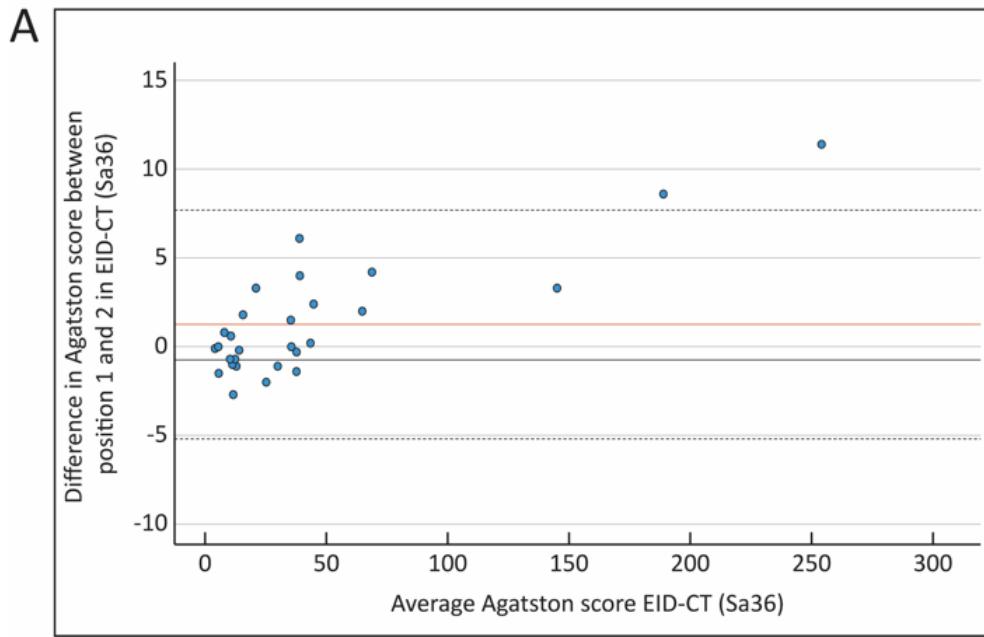


Figure 4

Bland-Altman plot for the energy integrating detector CT (EID-CT) (Sa36) (A). The solid red line shows the mean difference (1.26) and the dashed lines indicate +/- 2 SD (7.7 to -5.2). Bland-Altman plot for the photon counting detector CT PCD-CT (Qr36) (B). The solid red line shows mean difference (0.14) and the dashed lines indicate +/- 2 SD (8.4 to -8.1).

Supplementary Files

This is a list of supplementary files associated with this preprint. Click to download.

- ASforalllesions.docx